

TÜRK LOYDU



SHIPBUILDING AND REPAIR QUALITY STANDARD

2013

This latest edition incorporates all rule changes. The latest revisions are shown with a vertical line. The section title is framed if the section is revised completely. Changes after the publication of the rule are written in red colour.

Unless otherwise specified, these Rules apply to ships for which the date of contract for construction as defined in IACS PR No.29 is on or after 5th of October 2013. New rules or amendments entering into force after the date of contract for construction are to be applied if required by those rules. See Rule Change Notices on TL website for details.

"General Terms and Conditions" of the respective latest edition will be applicable (see Rules for Classification and Surveys).

If there is a difference between the rules in English and in Turkish, the rule in English is to be considered as valid. This publication is available in print and electronic pdf version. Once downloaded, this document will become UNCONTROLLED. Please check the website below for the valid version.

<http://www.turkloydu.org>

All rights are reserved by Türk Loydu, and content may not be reproduced, disseminated, published, or transferred in any form or by any means, except with the prior written permission of TL.

TÜRK LOYDU

Head Office Postane Mah. Tersaneler Cad. No:26 Tuzla 34944 İSTANBUL / TÜRKİYE
Tel : (90-216) 581 37 00
Fax : (90-216) 581 38 00
E-mail : info@turkloydu.org
<http://www.turkloydu.org>

Regional Offices

Ankara Eskişehir Yolu Mustafa Kemal Mah. 2159. Sokak No : 6/4 Çankaya - ANKARA / TÜRKİYE
Tel : (90-312) 219 56 34
Fax : (90-312) 219 68 25
E-mail : ankara@turkloydu.org

İzmir Atatürk Cad. No :378 K.4 D.402 Kavalalılar Apt. 35220 Alsancak - İZMİR / TÜRKİYE
Tel : (90-232) 464 29 88
Fax : (90-232) 464 87 51
E-mail : izmir@turkloydu.org

Adana Çınarlı Mah. Atatürk Cad. Aziz Naci İş Merkezi No:5 K.1 D.2 Seyhan - ADANA / TÜRKİYE
Tel : (90- 322) 363 30 12
Fax : (90- 322) 363 30 19
E-mail : adana@turkloydu.org

Shipbuilding and Repair Quality Standard

Page

Section 1 – Shipbuilding and Remedial Quality Standard for New Construction

A. Scope	1- 2
B. General Requirements for New Construction.....	1- 2
C. Qualification of Personnel and Procedures.....	1- 3
D. Materials	1- 3
E. Gas Cutting.....	1- 5
F. Fabrication and Fairness	1- 5
G. Alignment.....	1- 6
H. Welding Joint Details	1- 6
I. Remedial	1- 6

Section 2 – Repair Quality Standard for Existing Ships

A. Scope	2- 2
B. General Requirements to Repairs and Repairers	2- 2
C. Qualification of Personnel.....	2- 2
D. Materials	2- 3
E. General Requirements to Welding.....	2- 4
F. Repair Quality Standard	2- 8

AMENDMENTS

Revised Sections	RCS No.	EIF Date*
Section 01	01/2018	01.01.2018
Section 02	01/2018	01.01.2018
Section 01	01/2017	01.01.2017

* Entry into Force (EIF) Date is provided for general guidance only, EIF dates given in Rule Change Summary (RCS) are considered valid. In addition to the above stated changes, editorial corrections may have been made.

SECTION 1

SHIPBUILDING AND REMEDIAL QUALITY STANDARD FOR NEW CONSTRUCTION

	Page
A. SCOPE	1- 2
B. GENERAL REQUIREMENTS FOR NEW CONSTRUCTION	1- 2
C. QUALIFICATION OF PERSONNEL AND PROCEDURES	1- 3
1. Qualification of welders	
2. Qualification of welding procedures	
3. Qualification of NDE operators	
D. MATERIALS	1- 3
1. Materials for structural members	
2. Surface conditions	
E. GAS CUTTING	1- 5
F. FABRICATION AND FAIRNESS	1- 5
1. Flanged longitudinals and flanged brackets	
2. Built-up sections	
3. Corrugated bulkheads	
4. Pillars, brackets and stiffeners	
5. Maximum heating temperature on surface for line heating	
6. Block assembly	
7. Special sub-assembly	
8. Shape	
9. Fairness of plating between frames	
10. Fairness of plating with frames	
11. Preheating for welding hull steels at low temperature	
G. ALIGNMENT	1- 6
H. WELDING JOINT DETAILS	1- 6
1. Typical butt weld plate edge preparation (manual welding and semi-automatic welding)	
2. Typical fillet weld plate edge preparation (manual welding and semi-automatic welding)	
3. Butt and fillet weld profile (manual welding and semi-automatic welding)	
4. Typical butt weld edge preparation (Automatic welding)	
5. Distance between welds	
I. REMEDIAL	1- 6
1. Typical misalignment remedial	
2. Typical butt weld plate edge preparation remedial (manual welding and semi-automatic welding)	
3. Typical fillet weld plate edge preparation remedial (manual welding and semi-automatic welding)	
4. Typical fillet and butt weld profile remedial (manual welding and semi-automatic welding)	
5. Distance between welds remedial	
6. Erroneous hole remedial	
7. Remedial by insert plate	
8. Weld surface remedial	
9. Weld remedial (short bead)	

A. Scope

1. This standard provides guidance on shipbuilding quality standards for the hull structure during new construction and the remedial standard where the quality standard is not met.

Whereas the standard generally applies to

- Conventional merchant ship types,
- Parts of hull covered by the rules of **TL**,
- Hull structures constructed from normal and higher strength hull structural steel,

the applicability of the standard is in each case to be agreed upon by **TL**.

The standard does generally not apply to the new construction of

- Special types of ships as e.g. gas tankers,
- Structures fabricated from stainless steel or other, special types or grades of steel.

2. In this standard, both a "Standard" range and a "Limit" range are listed. The "Standard" range represents the target range expected to be met in regular work under normal circumstances. The "Limit" range represents the maximum allowable deviation from the "Standard" range. Work beyond the "Standard" range but within the "Limit" range is acceptable. In cases where no 'limit' value is specified, the value beyond the 'standard' range may be accepted subject to the consideration of **TL**.

3. The standard covers typical construction methods and gives guidance on quality standards for the most important aspects of such construction. Unless explicitly stated elsewhere in the standard, the level of workmanship reflected herein will in

principle be acceptable for primary and secondary structure of conventional designs. A more stringent standard may however be required for critical and highly stressed areas of the hull, and this is to be agreed with **TL** in each case. **In assessing the criticality of hull structure and structural components, reference is made to ref. A1, A2, A3, A11, A15, A16 and A17.**

4. Details relevant to structures or fabrication procedures not covered by this standard are to be approved by **TL** on the basis of procedure qualifications and/or recognized national standards.

5. For use of this standard, fabrication fit-ups, deflections and similar quality attributes are intended to be uniformly distributed about the nominal values. The shipyard is to take corrective action to improve work processes that produce measurements where a skew distribution is evident. Relying upon remedial steps that truncate a skewed distribution of the quality attribute is unacceptable.

B. General Requirements for New Construction

1. In general, the work is to be carried out in accordance with **TL** rules and under the supervision of the Surveyor to **TL**.

2. Welding operations are to be carried out in accordance with work instructions accepted by **TL**.

3. Welding of hull structures is to be carried out by qualified welders, according to approved and qualified welding procedures and with welding consumables approved by **TL**, see item C. Welding operations are to be carried out under proper supervision by the shipbuilder. The working conditions for welding are to be monitored by **TL** in accordance with IACS, UR Z23 (ref. A12).

C. Qualification of Personnel and Procedures

1. Qualification of Welders

1.1 Welders are to be qualified in accordance with the procedures of **TL** or to a recognized national or international standard. Recognition of other standards is subject to submission to **TL** for evaluation. Subcontractors are to keep records of welders qualification and, when required, furnish valid approval test certificates.

1.2 Welding operators using fully mechanized or fully automatic processes need generally not pass approval testing provided that the production welds made by the operators are of the required quality. However, operators are to receive adequate training in setting or programming and operating the equipment. Records of training and operation experience shall be maintained on individual operator's files and records, and be made available to **TL** for inspection when requested.

2. Qualification of Welding Procedures

Welding procedures are to be qualified in accordance with IACS, URW28 (ref. A10) or other recognized standard accepted by **TL**.

3. Qualification of NDE operators

Personnel performing non-destructive examination for the purpose of assessing quality of welds in connection with new construction covered by this standard, are to be qualified in accordance with **TL** rules or to a recognized international or national qualification scheme. Records of operators and their current certificates are to be kept and made available to the Surveyor for inspection.

D. Materials

1. Materials for Structural Members

All materials, including weld consumables, to be used for

the structural members are to be approved by **TL** as per the approved construction drawings and meet the respective IACS Unified Requirements (see ref. A4, A5, A6, A7, A8 and A9) Additional recommendations are contained in the following paragraphs.

All materials used should be manufactured at a works approved by **TL** for the type and grade supplied.

2. Surface Conditions

2.1 Definitions

Minor Imperfections : Pitting, rolled-in scale, indentations, roll marks, scratches and groove

Defects, : Shells, sand patches, sharp edged seams and minor imperfections exceeding the limits of Table 1.1

Depth of imperfections or defects : The depth is to be measured from the surface of the product

2.2 Acceptance without remedies

Minor imperfections, in accordance with the nominal thickness (t) of the product and the limits described in Table 1.1, are permissible and may be left as they are.

Imperfection surface area Ratio (%) is obtained as influenced area / area under consideration (i.e. plate surface area) x 100%.

For isolated surface discontinuities, influenced area is obtained by drawing a continuous line which follows the circumference of the discontinuity at a distance of 20 mm. (Figure 1.1)

Table 1.1 Limits for depth of minor imperfection, for acceptance without remedies

Imperfection surface area Ratio(%)	15 ~ 20%	5 ~ 15%	0 ~ 5%
$t < 20 \text{ mm}$	0.2 mm	0.4 mm	0.5 mm
$20 \text{ mm} \leq t < 50 \text{ mm}$	0.2 mm	0.6 mm	0.7 mm
$50 \text{ mm} \leq t$	0.2 mm	0.7 mm	0.9 mm

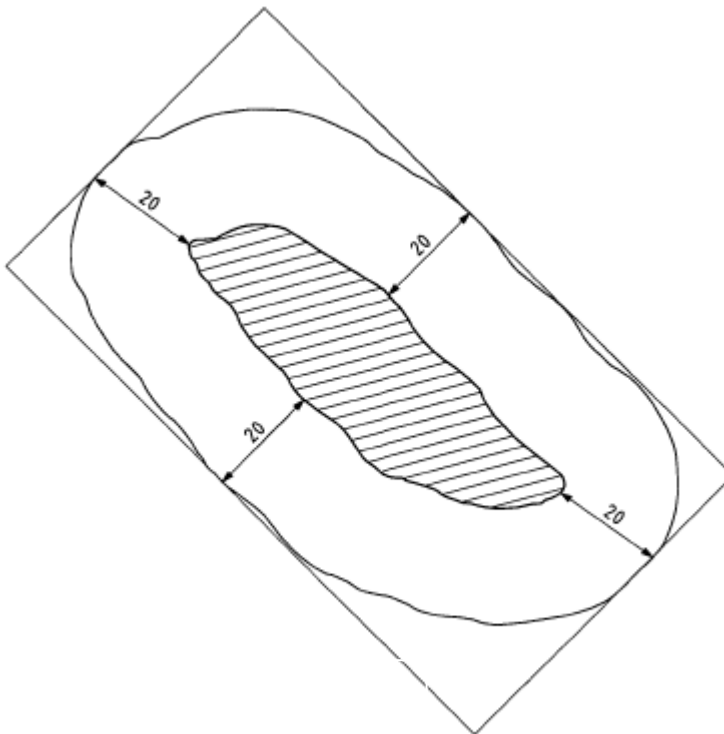


Figure 1.1 - Determination of the area influenced by an isolated discontinuity
(Ref. Nr. EN 10163-1:2004+AC:2007 E)

For surface discontinuities appearing in a cluster, influenced area is obtained by drawing a continuous line which follows the circumference of the cluster at a distance of 20 mm. (Figure 1.2)

2.3 Remedial of Defects

Defects are to be remedied by grinding and/or welding in accordance with IACS Rec.12 (ref. A12).

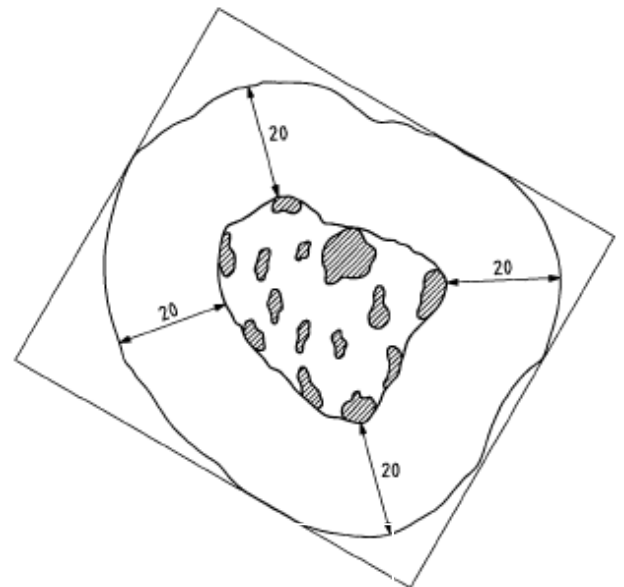


Figure 1.2 - Determination of the area influenced by clustered discontinuities
(Ref. Nr. EN 10163-1:2004+AC:2007 E)

2.4 Further Defects

2.4.1 Lamination

Investigation to be carried out at the steelmill into the cause and extent of the detected laminations. Severe lamination is to be remedied by local insert plates. The minimum breadth or length of the plate to be replaced is to be:

- 1600 mm for shell and strength deck plating in way of cruciform or T-joints,

- 800 mm for shell, strength deck plating and other primary members,
- 300 mm for other structural members.

Local limited lamination may be remedied by chipping and/or grinding followed by welding in accordance with Figure 1.3. In case where the local limited lamination is near the plate surface, the remedial may be carried out as shown in Figure 1.4. For limitations see item 2.2.

2.4.2 Weld Spatters

Loose weld spatters are to be removed by grinding or other measures to clean metal surface (see Table 1.26), as required by the paint system, on:

- Shell plating,
- Deck plating on exposed decks,
- In tanks for chemical cargoes,
- In tanks for fresh water and for drinking water,
- In tanks for lubricating oil, hydraulic oil, including service tanks.

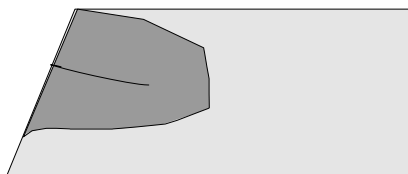


Figure 1.3

E. Gas Cutting

The roughness of the cut edges is to meet the following requirements:

Free Edges:

	Standard	Limit
Strength Members	150 μm	300 μm
Others	500 μm	1000 μm

Welding Edges:

	Standard	Limit
Strength Members	400 μm	800 μm
Others	800 μm	1500 μm

F. Fabrication and Fairness

1. Flanged longitudinals and flanged brackets (see Table 1.2).
2. Built-up sections (see Table 1.3).
3. Corrugated bulkheads (see Table 1.4).
4. Pillars, brackets and stiffeners (see Table 1.5).
5. Maximum heating temperature on surface for line heating (see Table 1.6).

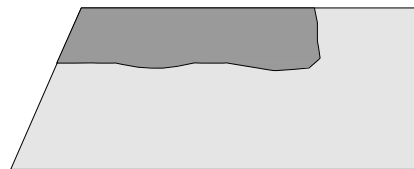


Figure 1.4

6. Block assembly (see Table 1.7).
7. Special sub-assembly (see Table 1.8).
8. Shape (see Table 1.9).
9. Fairness of plating between frames (see Table 1.10).
10. Fairness of plating with frames (see Table 1.11).
11. Preheating for welding hull steels at low temperature (see Table 1.12).

G. Alignment

The quality standards for alignment of hull structural components during new construction are shown in Table 1.13. TL may require a closer construction tolerance in areas requiring special attention, as follows:

- Regions exposed to high stress concentrations
- Fatigue prone areas
- Detail design block erection joints
- High tensile steel regions

H. Welding Joint Details

Edge preparation is to be qualified in accordance with IACS, URW28 (ref. A10) or other recognized standard accepted by TL.

Some typical edge preparations are shown in Table 1.14, 1.15 and 1.17 for reference.

1. Typical butt weld plate edge preparation (manual and semi-automatic welding) for reference, see Table 1.14
2. Typical fillet weld plate edge preparation (manual and semi-automatic welding) for reference, see Table 1.15

3. Butt and fillet weld profile (manual and semi-automatic welding), see Table 1.16
4. Typical butt weld plate edge preparation (Automatic welding) for reference, see Table 1.17.
5. Distance between welds, see Table 1.18.

I. Remedial

All the major remedial work is subject to reporting by shipbuilder to TL for approval in accordance with their work instruction for new building.

Some typical remedial works are shown in Table 1.19.

1. Typical misalignment remedial, see Table 1.19.
2. Typical butt weld plate edge preparation remedial (manual and semi-automatic welding), see Table 1.20.
3. Typical fillet weld plate edge preparation remedial (manual and semi-automatic welding), see Table 1.21.
4. Typical fillet and butt weld profile remedial (manual and semi-automatic welding), see Table 1.22.
5. Distance between welds remedial, see Table 1.23.
6. Erroneous hole remedial, see Table 1.24.
7. Remedial by insert plate, see Table 1.25.
8. Weld surface remedial, see Table 1.26.
9. Weld remedial (short bead), see Table 1.27.

Table 1.2 Flanged longitudinals and flanged brackets



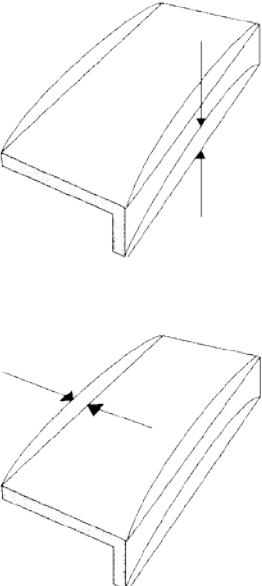
Detail	Standard	Limit	Remarks
<p>Breadth of flange</p>  <p>compared to correct size</p>	± 3 mm	± 5 mm	
<p>Angle between flange and web</p>  <p>compared to template</p>	± 3 mm	± 5 mm	per 100 mm of a
<p>Straightness in plane of flange and web</p> 	± 10 mm	± 25 mm	per 10 m

Table 1.3 Built up sections

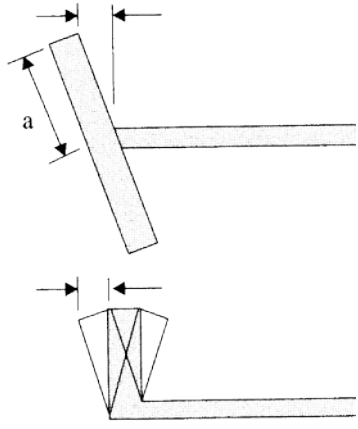
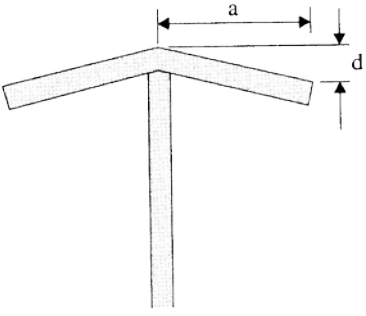
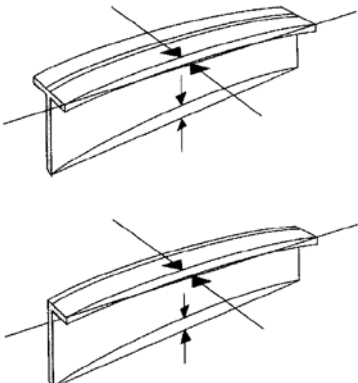

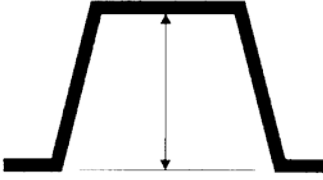
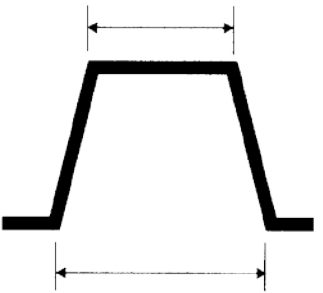
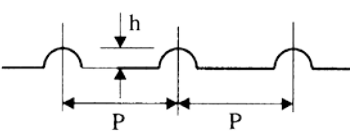
Detail	Standard	Limit	Remarks
<p>Frames and longitudinal</p> 	$\pm 1.5 \text{ mm}$	$\pm 3 \text{ mm}$	per 100 mm of a
<p>Distortion of face plate</p> 	$d \leq 3 + a/100 \text{ mm}$	$d \leq 5 + a/100 \text{ mm}$	
<p>Distortion in plane of web and flange of built up longitudinal frame, transverse frame, girder and transverse web.</p> 	$\pm 10 \text{ mm}$	$\pm 25 \text{ mm}$	per 10 m in length

Table 1.4 Corrugated bulkheads

Detail	Standard	Limit	Remarks
Mechanical bending 	$R \geq 3t$ mm $R \geq 4.5t$ mm for CSR ships (1)	$2t$ mm(2)	Material to be suitable for cold flanging (forming) and welding in way of radius
Depth of corrugation 	± 3 mm	± 6 mm	
Breadth of corrugation 	± 3 mm	± 6 mm	
Pitch and depth of swedged corrugated bulkhead compared with correct value 	$h : \pm 2.5$ mm Where it is not aligned with other bulkheads $P : \pm 6$ mm Where it is aligned with other bulkheads $P : \pm 2$ mm	$h : \pm 5$ mm Where it is not aligned with other bulkheads $P : \pm 9$ mm Where it is aligned with other bulkheads $P : \pm 3$ mm	

Notes for Table 1.4

(1) For CSR Bulk Carriers built under the “Common Structural Rules for Bulk Carriers” with the effective dates of 1 July 2010 and 1 July 2012, the standard is $R \geq 2t$ mm.

(2) For CSR ships, the allowable inside bending radius of cold formed plating may be reduced provided the following requirements are complied with.

When the inside bending radius is reduced below 4.5 times the as-built plate thickness, supporting data is to be provided. The bending radius is in no case to be less than 2 times the as-built plate thickness. As a minimum, the following additional requirements are to be complied with:

a) For all bent plates:

- 100% visual inspection of the bent area is to be carried out.
- Random checks by magnetic particle testing are to be carried out.

b) In addition to a), for corrugated bulkheads subject to lateral liquid pressure:

- The steel is to be of Grade D/DH or higher.

The material is impact tested in the strain-aged condition and satisfies the requirements stated herein. The deformation is to be equal to the maximum deformation to be applied during production, calculated by the formula $t_{as-built} / (2r_{bdg} + t_{as-built})$, where $t_{as-built}$ is the as-built thickness of the plate material and r_{bdg} is the bending radius. One sample is to be plastically strained at the calculated deformation or 5%, whichever is greater and then artificially aged at 250°C for one hour then subject to Charpy V-notch testing. The average impact energy after strain ageing is to meet the impact requirements specified for the grade of steel used.

Table 1.5 Pillars, brackets and stiffeners

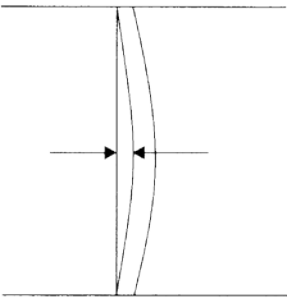

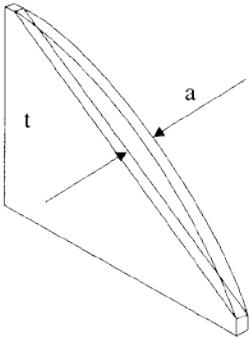

Detail	Standard	Limit	Remarks
Pillar (between decks) 	4 mm	6 mm	
Cylindrical structure diameter (pillars, masts, posts, etc.) 	$\pm D/200$ mm max. + 5 mm	$\pm D/150$ mm max. 7.5 mm	
Tripping bracket and small stiffener, distortion at the part of free edge 	$a \leq t/2$ mm	t	
Ovality of cylindrical structure 		$d_{\max} - d_{\min} \leq 0.02 \times d_{\max}$	

Table 1.6 Maximum Heating Temperature on Surface for Line Heating

Item		Standard	Limit	Remarks
Conventional Process AH32-EH32 & AH36-EH36	Water cooling just after heating	Under 650°C		
	Air cooling after heating	Under 900°C		
	Air cooling and subsequent water cooling after heating	Under 900°C (starting temperature of water cooling to be under 500°C)		
TMCP type AH32-EH36 (Ceq.>0.38%)				
TMCP type AH32-DH32 & AH36-DH36 (Ceq. ≤ 0.38%)	Water cooling just after heating or air cooling	Under 1000°C		
	Water cooling just after heating or air cooling	Under 900°C		
TMCP type EH32 & EH36 (Ceq. ≤ 0.38%)				
<p><i>Note:</i></p> $Ceq = C + \frac{Mn}{6} + \frac{Cr + Mo + V}{5} + \frac{Ni + Cu}{15} (\%)$				

Table 1.7 Block assembly

Item	Standard	Limit	Remarks
Flat Plate Assembly			
Length and Breadth	± 4 mm	± 6 mm	
Distortion	± 10 mm	±20mm	
Squareness	± 5 mm	±10mm	
Deviation of interior members from plate	5 mm	10mm	
Curved plate assembly			
Length and Breadth	± 4 mm	± 8 mm	measured along the girth
Distortion	± 10 mm	± 20 mm	
Squareness	± 10 mm	± 15 mm	
Deviation of interior members from plate	5 mm	10 mm	
Flat cubic assembly			
Length and Breadth	± 4 mm	± 6 mm	
Distortion	± 10 mm	± 20 mm	
Squareness	± 5 mm	± 10 mm	
Deviation of interior members from plate	5 mm	10 mm	
Twist	± 10 mm	± 20 mm	
Deviation between upper and lower plate	± 5 mm	± 10 mm	
Curved cubic assembly			
Length and Breadth	± 4 mm	± 8 mm	measured along with girth
Distortion	± 10 mm	± 20 mm	
Squareness	± 10 mm	± 15 mm	
Deviation of interior members from plate	± 5 mm	± 10 mm	
Twist	± 15 mm	± 25 mm	
Deviation between upper and lower plate	± 7 mm	± 15 mm	

Table 1.8 Special Sub-Assembly

Item	Standard	Limit	Remarks
Distance between upper/lower gudgeon	± 5 mm	± 10 mm	
Distance between aft edge of boss and aft peak bulkhead	± 5 mm	± 10 mm	
Twist of sub-assembly of stern frame	5 mm	10 mm	
Deviation of rudder from shaft center line	4 mm	8 mm	
Twist of rudder plate	6 mm	10 mm	
Flatness of top plate of main engine bed	5 mm	10 mm	
Breadth and length of top plate of main engine bed	± 4 mm	± 6 mm	
<p>Note: Dimensions and tolerances have to fulfill engine and equipment manufacturers' requirements, if any.</p>			

Table 1.9 Shape



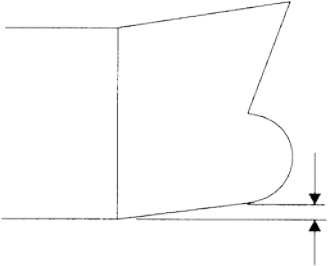
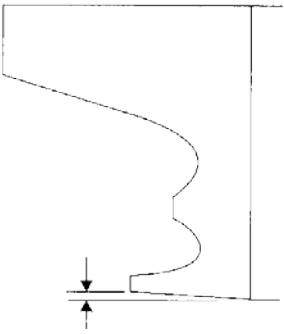
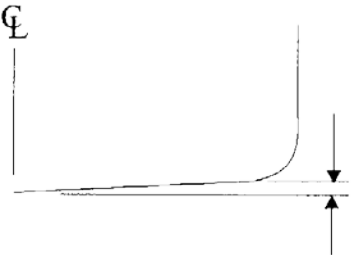
Detail	Standard	Limit	Remarks
Deformation for the whole length 	± 50 mm		per 100 m against the line of keel sighting
Deformation for the distance between two adjacent bulkheads 	± 15 mm		
Cocking-up of fore body 	± 30 mm		The deviation is to be measured from the design line.
Cocking-up of aft-body 	± 20 mm		
Rise of floor amidships 	± 15 mm		The deviation is to be measured from the design line.

Table 1.9 Shape (cont.)

Item	Standard	Limit	Remarks
Length between perpendiculars	$\pm L/1000$ mm where L is in mm		Applied to ships of 100 metre length and above. For the convenience of the measurement the point where the keel is connected to the curve of the stem may be substituted for the fore perpendicular in the measurement of the length.
Moulded breadth at midship	$\pm B/1000$ mm where B is in mm		Applied to ships of 15 metre breadth and above, measured on the upper deck.
Moulded depth at midship	$\pm D/1000$ mm where D is in mm		Applied to ships of 10 metre depth and above, measured up to the upper deck.

Table 1.10 Fairness of plating between frames


Item		Standard	Limit	Remarks
Shell plate	Parallel part (side & bottom shell)	4 mm	8 mm	
	Fore and aft part	5 mm		
Tank top plate	4 mm			
Bulkhead	Longl. Bulkhead	6 mm	8 mm	
	Trans. Bulkhead			
	Swash Bulkhead			
Strength deck	Parallel part	4 mm	8 mm	
	Fore and aft part	6 mm	9 mm	
	Covered part	7 mm	9 mm	
Second deck	Bare part	6 mm	8 mm	
	Covered part	7 mm	9 mm	
Forecastle deck poop deck	Bare part	4 mm	8 mm	
	Covered part	6 mm	9 mm	
Super structure deck	Bare part	4 mm	6 mm	
	Covered part	7 mm	9 mm	
House wall	Outside wall	4 mm	6 mm	
	Inside wall	6 mm	8 mm	
	Covered part	7 mm	9 mm	
Interior member (web of girder, etc)		5 mm	7 mm	
Floor and girder in double bottom		5 mm	8 mm	

Table 1.11 Fairness of plating with frames

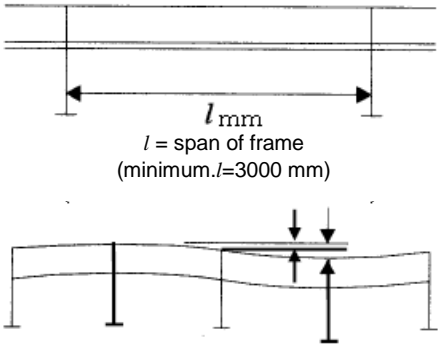
Item		Standard	Limit	Remarks
Shell plate	Parallel part	$\pm 2 l / 1000$ mm	$\pm 3 l / 1000$ mm	$l =$ span of frame To be measured between on trans. space (min. $l=3000$ mm)
	Fore and aft part	$\pm 3 l / 1000$ mm	$\pm 4 l / 1000$ mm	
Strength deck (excluding cross deck) and top plate of double bottom	-	$\pm 3 l / 1000$ mm	$\pm 4 l / 1000$ mm	
Bulkhead	-		$\pm 5 l / 1000$ mm	
Accommodation above the strength deck and others	-	$\pm 5 l / 1000$ mm	$\pm 6 l / 1000$ mm	
 <p>To be measured between one trans. space.</p>				

Table 1.12 Preheating for welding hull steels at low temperature

Item		Standard		Limit	Remarks
		Base metal temperature needed preheating	Minimum preheating temperature		
Normal strength steels	A, B, D, E	Below -5 °C	20 °C (1)		
Higher strength steels (TMCP type)	AH32 – EH32 AH36 – EH36	Below 0 °C			
Higher strength steels (Conventional type)		Below 0 °C			
Note: (1) This level of preheat is to be applied unless the approved welding procedure specifies a higher level.					

Table 1.13 Alignment

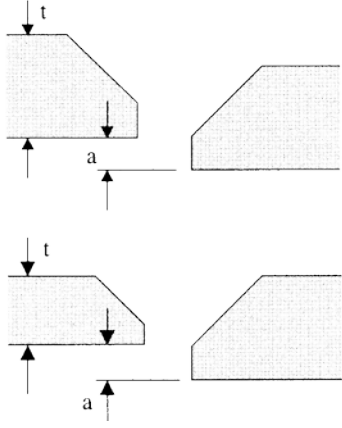
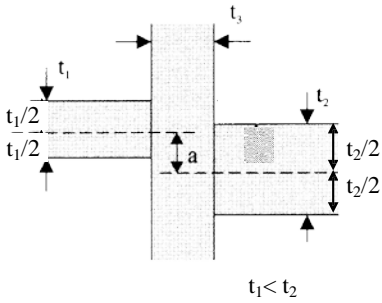
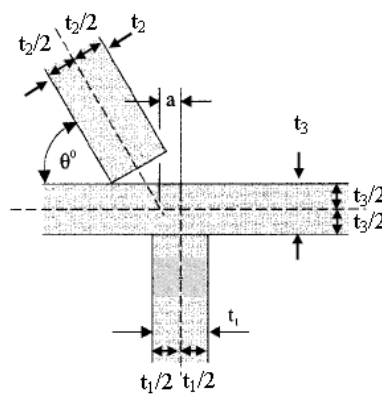
Detail	Standard	Limit	Remarks
<p>Alignment of butt welds</p> 		<p>$a \leq 0.15t$ strength member $a \leq 0.2t$ other but maximum 4.0 mm</p>	<p>t is the lesser plate thickness</p>
<p>Alignment of fillet welds</p>  <p>$t_1 < t_2$</p>		<p>Strength member and higher stress member: $a \leq t_1/3$</p> <p>Other: $a \leq t_1/2$</p>	<p>Alternatively, heel line can be used to check the alignment.</p> <p>Where t_3 is less than t_1, then t_3 should be substituted for t_1 in the standard.</p>
<p>Alignment of fillet welds</p> 		<p>Strength member and higher stress member: $a \leq t_1/3$</p> <p>Other: $a \leq t_1/2$</p>	<p>Alternatively, heel line can be used to check the alignment.</p> <p>Where t_3 is less than t_1, then t_3 should be substitute for t_1 in the standard.</p>

Table 1.13 Alignment (cont.)

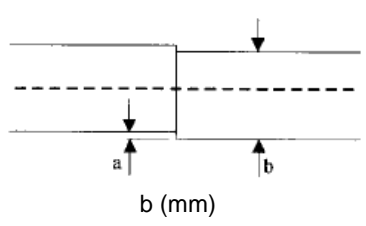
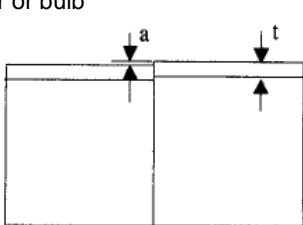
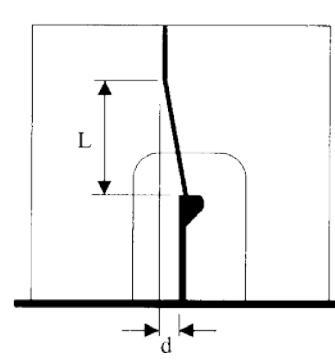
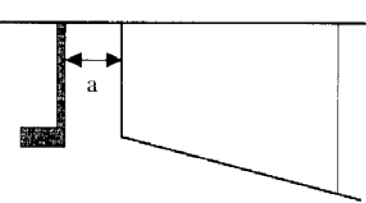
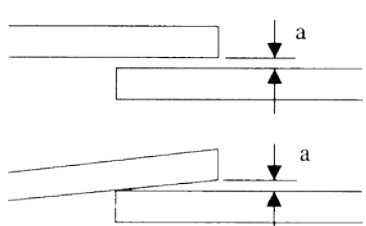
Detail	Standard	Limit	Remarks
<p>Alignment of flange of T-longitudinal</p> 	<p>Strength member $a \leq 0.04b$ (mm)</p>	<p>$a = 8.0$ mm</p>	
<p>Alignment of height of T-bar, L-angle bar or bulb</p> 	<p>Strength member $a \leq 0.15t$</p> <p>Other $a \leq 0.20t$</p>	<p>$a = 3.0$ mm</p>	
<p>Alignment of panel stiffener</p> 	<p>$d \leq L/50$</p>		
<p>Gap between bracket/intercostal and stiffener</p> 	<p>$a \leq 2.0$ mm</p>	<p>$a = 3.0$ mm</p>	
<p>Alignment of lap welds</p> 	<p>$a \leq 2.0$ mm</p>	<p>$a = 3.0$ mm</p>	

Table 1.13 Alignment (cont.)

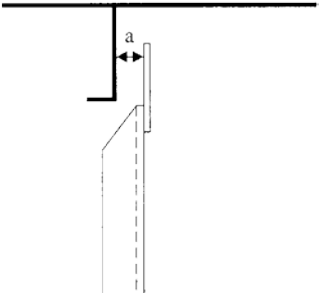
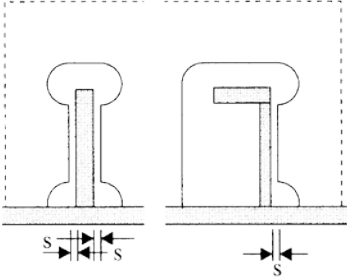
Detail	Standard	Limit	Remarks
<p data-bbox="172 315 501 344">Gap between beam and frame</p> 	$a \leq 2.0 \text{ mm}$	$a = 5.0 \text{ mm}$	
<p data-bbox="172 801 480 831">Gap around stiffener cut-out</p> 	$s \leq 2.0 \text{ mm}$	$s = 3.0 \text{ mm}$	

Table 1.14 Typical Butt Weld Plate Edge Preparation (Manual Welding and Semi-Automatic Welding) for Reference

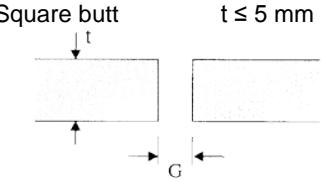
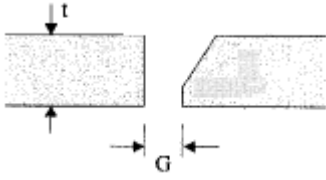
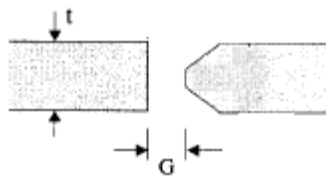
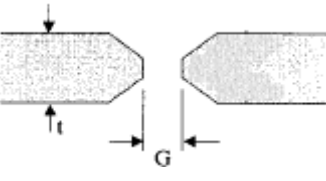
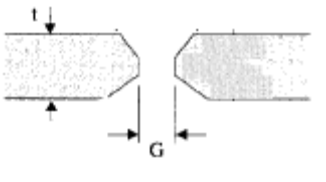
Detail	Standard	Limit	Remarks
Square butt $t \leq 5$ mm 	$G \leq 3$ mm	$G = 5$ mm	see Note
Single bevel butt $t > 5$ mm 	$G \leq 3$ mm	$G = 5$ mm	see Note
Double bevel butt $t > 19$ mm 	$G \leq 3$ mm	$G = 5$ mm	see Note
Double vee butt, uniform bevels 	$G \leq 3$ mm	$G = 5$ mm	see Note
Double vee butt, non-uniform bevel 	$G \leq 3$ mm	$G = 5$ mm	see Note
<p>Note : Different plate edge preparation may be accepted or approved by TL in accordance with URW28 (ref. A10) or other recognized standard accepted by TL. For welding procedures other than manual welding, see C, 2. Qualification of weld procedures.</p>			

Table 1.14 Typical Butt Weld Plate Edge Preparation (Manual Welding and Semi-Automatic Welding) for Reference (cont.)

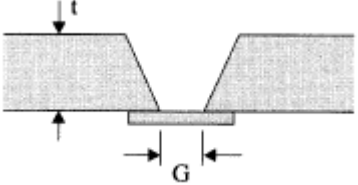
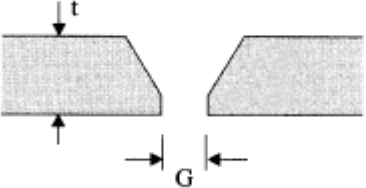
Detail	Standard	Limit	Remarks
<p>Single Vee butt, one side welding with backing strip (temporary or permanent)</p> 	<p>$G = 3 \text{ to } 9 \text{ mm}$</p>	<p>$G = 16 \text{ mm}$</p>	<p>see Note</p>
<p>Single vee butt</p> 	<p>$G \leq 3 \text{ mm}$</p>	<p>$G = 5 \text{ mm}$</p>	<p>see Note</p>
<p>Note : Different plate edge preparation may be accepted or approved by TL in accordance with URW28 (ref. A10) or other recognized standard accepted by TL. For welding procedures other than manual welding, see C.2. Qualification of welding procedures.</p>			

Table 1.15 Typical Fillet Weld Plate Edge Preparation (Manual Welding and Semi-Automatic Welding) for Reference

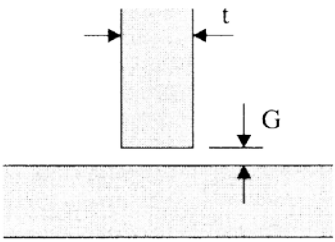
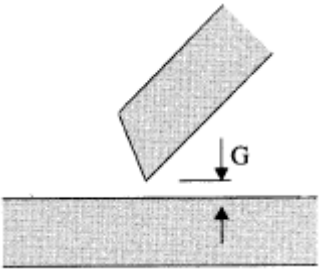
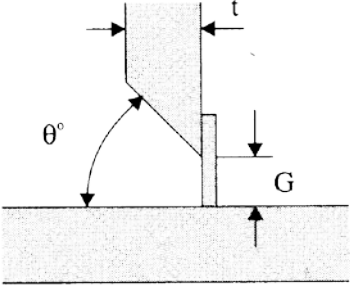
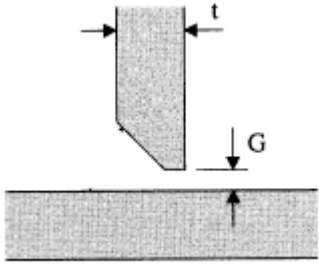
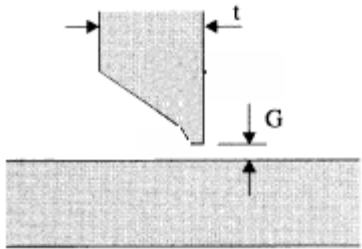
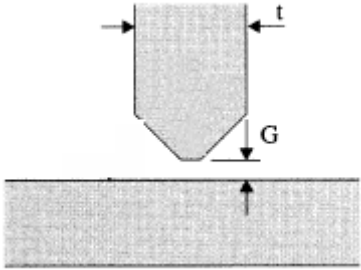
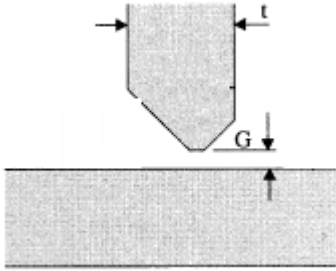
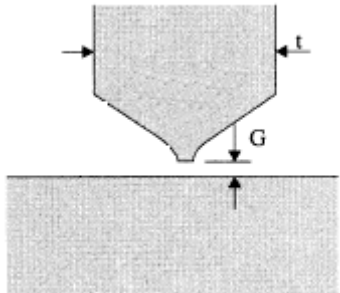
Detail	Standard	Limit	Remarks
<p>Tee Fillet</p> 	$G \leq 2 \text{ mm}$	$G = 3 \text{ mm}$	see Note
<p>Inclined fillet</p> 	$G \leq 2 \text{ mm}$	$G = 3 \text{ mm}$	see Note
<p>Single bevel tee with permanent backing</p> 	$G \leq 4 \text{ to } 6 \text{ mm}$ $\theta^\circ = 30^\circ \text{ to } 45^\circ$	$G = 16 \text{ mm}$	<p>Not normally for strength member</p> <p>also see Note</p>
<p>Single bevel tee</p> 	$G \leq 3 \text{ mm}$		see Note
<p>Note : Different plate edge preparation may be accepted or approved by TL in accordance with URW28 (ref. A10) or other recognized standard accepted by TL. For welding procedures other than manual welding, see C.2. Qualification of welding procedures.</p>			

Table 1.15 Typical Fillet Weld Plate Edge Preparation (Manual Welding and Semi-Automatic Welding) for Reference (cont.)

Detail	Standard	Limit	Remarks
Single 'J' bevel tee 	G = 2.5 to 4 mm		see Note
Double bevel tee symmetrical $t > 19$ mm 	$G \leq 3$ mm		see Note
Double bevel tee asymmetrical $t > 19$ mm 	$G \leq 3$ mm		see Note
Double 'J' bevel tee symmetrical 	G = 2.5 to 4 mm		see Note

Note :

Different plate edge preparation may be accepted or approved by **TL** in accordance with URW28 (ref. A10) or other recognized standard accepted by **TL**.

For welding procedures other than manual welding, see C, 2. Qualification of welding procedures.

Table 1.16 Butt And Fillet Weld Profile (Manual Welding and Semi-Automatic Welding)

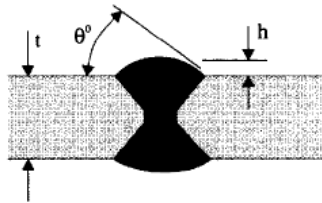
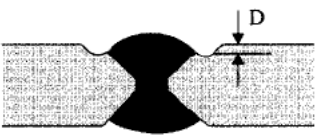

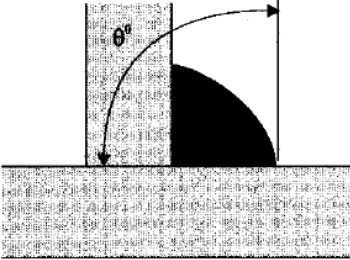
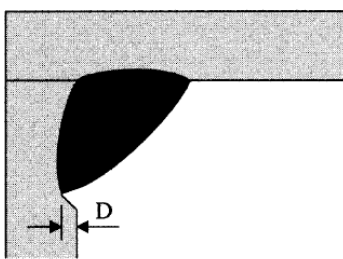
Detail	Standard	Limit	Remarks
Butt weld toe angle 	$\theta \leq 60^\circ$ $h \leq 6 \text{ mm}$	$\theta \leq 90^\circ$	
Butt weld undercut 		$D \leq 0.5 \text{ mm}$ for strength member $D \leq 0.8 \text{ mm}$ for other	
Fillet weld leg length  $s = \text{leg length}; a = \text{throat thickness}$		$s \geq 0.9s_d$ $a \geq 0.9a_d$ over short weld lengths	$s_d = \text{Design value for } s \text{ in mm.}$ $a_d = \text{Design value for } a \text{ in mm.}$
Fillet weld toe angle 		$\theta \leq 90^\circ$	
Fillet weld undercut 		$D \leq 0.8 \text{ mm}$	

Table 1.17 Typical Butt Weld Plate Edge Preparation (Automatic Welding) for Reference

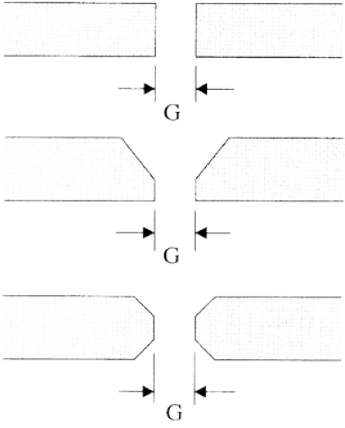
Detail	Standard	Limit	Remarks
<p data-bbox="172 309 512 340">Submerged Arc Welding (SAW)</p> 	$0 \leq G \leq 0.8 \text{ mm}$	$G = 2 \text{ mm}$	See Note.
<p data-bbox="172 853 236 875">Note :</p> <p data-bbox="172 880 1182 936">Different plate edge preparation may be accepted or approved by TL Society in accordance with URW28 (ref. A10) or other recognized standard accepted by TL.</p> <p data-bbox="172 936 1129 965">For welding procedures other than manual welding, see C, 2. Qualification of welding procedures.</p>			

Table 1.18 Distance Between Welds

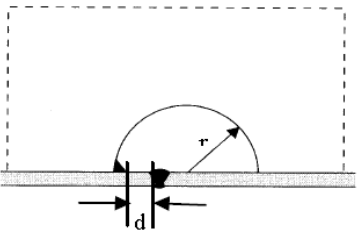
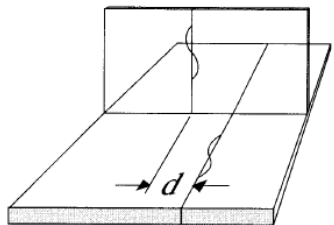
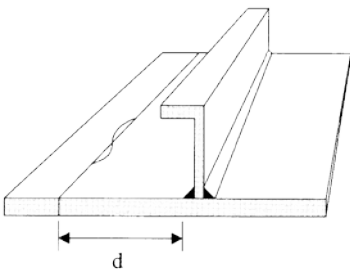
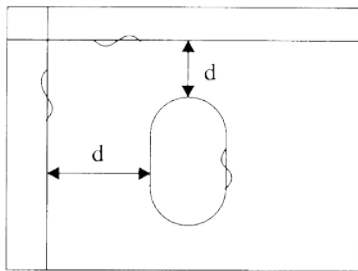
Detail	Standard	Limit	Remarks
<p>Scallops over weld seams</p> 		<p>for strength member $d \geq 5 \text{ mm}$</p> <p>for other $d \geq 0 \text{ mm}$</p>	<p>The "d" is to be measured from the toe of the fillet weld to the toe of the butt weld.</p>
<p>Distance between two butt welds</p> 		$d \geq 0 \text{ mm}$	
<p>Distance between butt weld and fillet weld</p> 		<p>for strength member $d \geq 10 \text{ mm}$</p> <p>for other $d \geq 0 \text{ mm}$</p>	<p>The "d" is to be measured from the toe of the fillet weld to the toe of the butt weld.</p>
<p>Distance between butt welds</p> 	<p>for cut-outs $d \geq 30 \text{ mm}$</p>		
	<p>for margin plates $d \geq 300 \text{ mm}$</p>	150 mm	

Table 1.19 Typical Misalignment Remedial

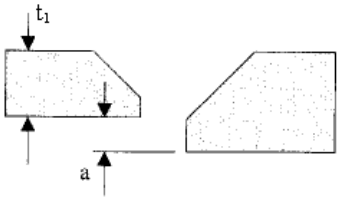
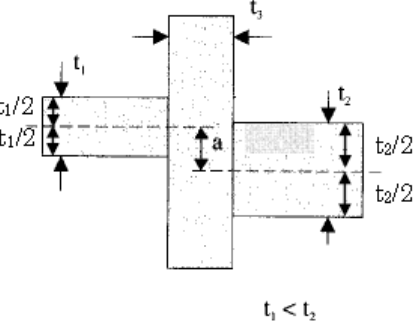
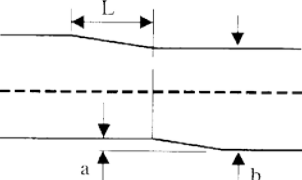
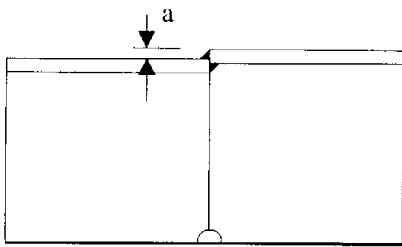
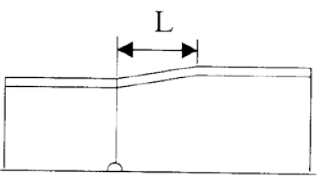
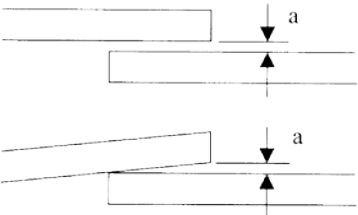
Detail	Remedial Standard	Remarks
<p>Alignment of butt joints</p> 	<p>Strength member $a > 0.15t_1$ or $a > 4$ mm release and adjust</p> <p>Other $a > 0.2t_1$ or $a > 4$ mm release and adjust</p>	<p>t_1 is lesser plate thickness</p>
<p>Alignment of fillet welds</p>  <p style="text-align: center;">$t_1 < t_2$</p>	<p>Strength member and higher stress member $t_1/3 < a \leq t_1/2$ - generally increase weld throat by 10%</p> <p>$a > t_1/2$- release and adjust over a minimum of 50a</p> <p>Other $a > t_1/2$- release and adjust over a minimum of 30a</p>	<p>Alternatively, heel line can be used to check the alignment.</p> <p>Where t_3 is less than t_1 then t_3 should be substituted for t_1 in standard</p>
<p>Alignment of flange of T-longitudinal</p> 	<p>When $0.04b < a \leq 0.08b$, max 8 mm: grind corners to smooth taper over a minimum distance $L = 3a$</p> <p>When $a > 0.08b$ or 8 mm: release and adjust over a minimum distance $L = 50a$</p>	
<p>Alignment of height of T-bar, L-angle bar or bulb</p> 	<p>When $3 \text{ mm} < a \leq 6 \text{ mm}$: build up by welding</p> <p>When $a > 6 \text{ mm}$: release and adjust over minimum $L = 50a$ for strength member and $L = 30a$ for other</p> 	
<p>Alignment of lap welds</p> 	<p>$3 \text{ mm} < a \leq 5 \text{ mm}$: weld leg length to be increased by the same amount as increase in gap in excess of 3 mm</p> <p>$a > 5 \text{ mm}$: members to be re-aligned</p>	

Table 1.19 Typical Misalignment Remedial (cont.)

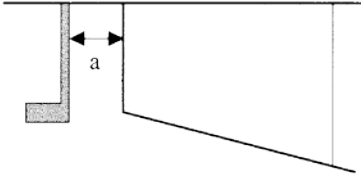
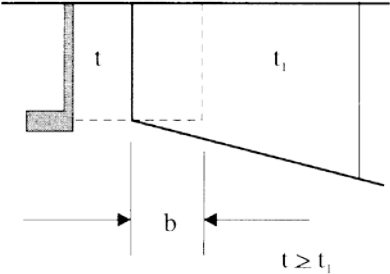
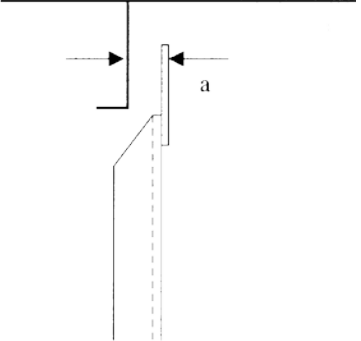
Detail	Remedial Standard	Remarks
<p data-bbox="172 315 576 371">Gap between bracket/intercostal and stiffener</p> 	<p data-bbox="624 315 1090 398">When $3 \text{ mm} < a \leq 5 \text{ mm}$: weld leg length to be increased by increase in gap in excess of 3 mm</p> <p data-bbox="624 412 1090 495">When $5 \text{ mm} < a \leq 10 \text{ mm}$: chamfer 30° to 40° and build up by welding with backing</p> <p data-bbox="624 508 1042 591">When $a > 10 \text{ mm}$: increase gap to about 50 mm and fit collar plate</p>  <p data-bbox="683 949 1002 981">$b = (2t + 25) \text{ mm, min. } 50 \text{ mm}$</p>	
<p data-bbox="172 1072 504 1104">Gap between beam and frame</p> 	<p data-bbox="624 1072 1046 1189">$3 \text{ mm} < a \leq 5 \text{ mm}$: weld leg length to be increased by the same amount as increase in gap in excess of 3 mm</p> <p data-bbox="624 1252 938 1283">$a > 5 \text{ mm}$ release and adjust</p>	

Table 1.19 Typical Misalignment Remedial (cont.)

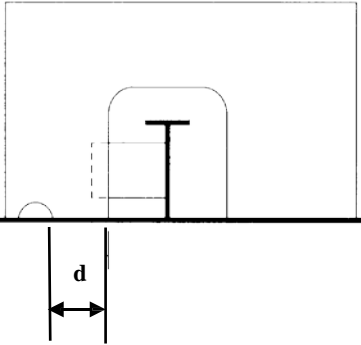
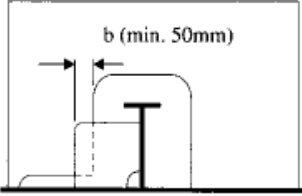

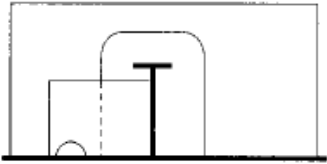
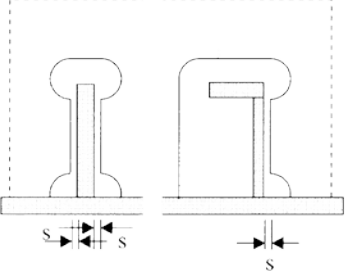

Detail	Remedial Standard	Remarks
<p>Position of scallop</p> 	<p>When $d < 75 \text{ mm}$ web plate to be cut between scallop and slot, and collar plate to be fitted</p>  <p>Or fit small collar over scallop</p>  <p>Or fit collar plate over scallop</p> 	
<p>Gap around stiffener cut-out</p> 	<p>When $3 \text{ mm} < s \leq 5 \text{ mm}$ weld leg length to be increased by the same amount as increase in gap in excess of 2 mm</p> <p>When $5 \text{ mm} < s \leq 10 \text{ mm}$ nib to be chamfered and built up by welding</p> <p>When $s > 10 \text{ mm}$ cut off nib and fit collar plate of same height as nib</p>  <p>$20 \text{ mm} \leq b \leq 50 \text{ mm}$</p>	

Table 1.20 Typical Butt Weld Plate Edge Preparation Remedial (Manual Welding and Semi-Automatic Welding)

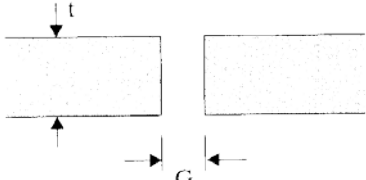
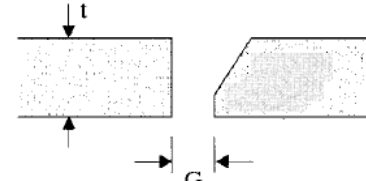

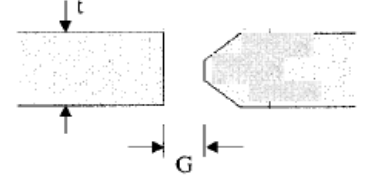
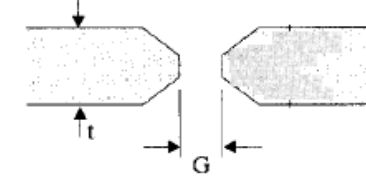
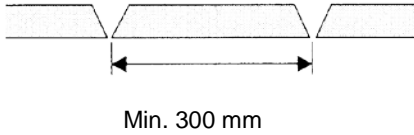
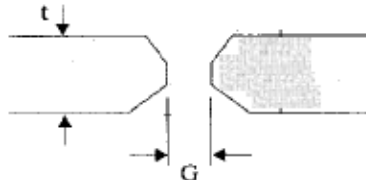
Detail	Remedial Standard	Remarks
<p>Square butt</p> 	<p>When $G \leq 10$ mm chamfer to 45° and build up by welding</p> <p>When $G > 10$ mm build up with backing strip; remove, back gouge and seal weld; or, insert plate, min. width 300 mm</p>	
<p>Single bevel butt</p> 	<p>When $5 \text{ mm} < G \leq 1.5t$ (maximum 25 mm) build up gap with welding on one or both edges to maximum of $0.5t$, using backing strip, if necessary.</p> <p>Where a backing strip is used, the backing strip is to be removed, the weld back gouged, and a sealing weld made.</p> 	
<p>Double bevel butt</p> 	<p>Different welding arrangement by using backing material approved by TL may be accepted on the basis of an appropriate welding procedure specification.</p> <p>When $G > 25$ mm or $1.5t$, whichever is smaller, use insert plate, of minimum width 300 mm</p>	
<p>Double vee butt, uniform bevels</p> 	 <p>Min. 300 mm</p>	
<p>Double vee butt, non-uniform bevel</p> 		

Table 1.20 Typical Butt Weld Plate Edge Preparation Remedial (Manual Welding and Semi-Automatic Welding) (cont.)

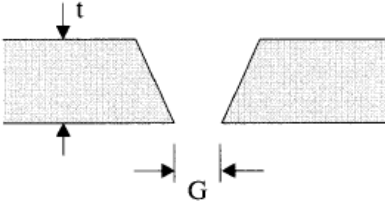
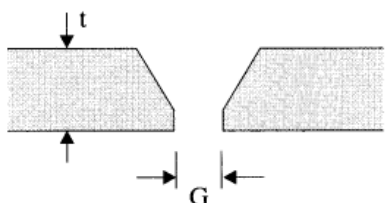
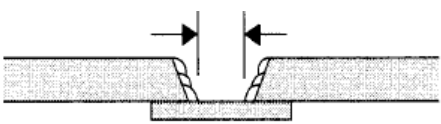
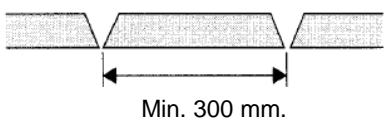
Detail	Remedial Standard	Remarks
<p>Single vee butt, one side welding</p> 	<p>When $5 \text{ mm} < G \leq 1.5t$ mm (maximum 25 mm), build up gap with welding on one or both edges, to "Limit" gap size preferably to "Standard" gap size as described in Table 1.14.</p> <p>Where a backing strip is used, the backing strip is to be removed, the weld back gouged, and a sealing weld made.</p> <p>Different welding arrangement by using backing material approved by TL may be accepted on the basis of an appropriate welding procedure specification.</p>	
<p>Single vee butt</p> 	<p>Limits see Table 1.14</p>  <p>When $G > 25 \text{ mm}$ or $1.5t$, whichever is smaller, use insert plate of minimum width 300 mm.</p>  <p>Min. 300 mm.</p>	

Table 1.21 Typical Fillet Weld Plate Edge Preparation Remedial (Manual Welding and Semi-Automatic Welding)

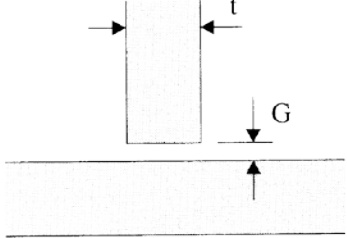
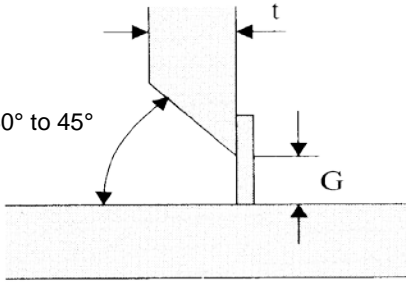
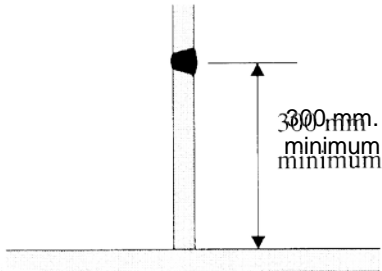
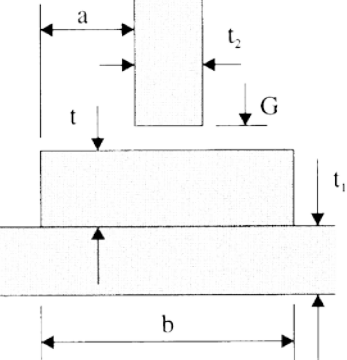
Detail	Remedial Standard	Remarks
	<p>$3 \text{ mm} < G \leq 5 \text{ mm}$ – leg length increased to Rule leg + (G-2)</p> <p>$5 \text{ mm} < G \leq 16 \text{ mm}$ or $G \leq 1.5t$ - chamfer by 30° to 45°, build up with welding, on one side, with backing strip if necessary, grind and weld.</p>  <p>$G > 16 \text{ mm}$ or $G > 1.5t$ use insert plate of minimum width 300 mm</p> 	
	<p>$t_2 \leq t \leq t_1$ $G \leq 2 \text{ mm}$ $a = 5 \text{ mm} + \text{fillet leg length}$</p>	<p>Not to be used in cargo area or areas of tensile stress through the thickness of the liner</p>

Table 1.21 Typical Fillet Weld Plate Edge Preparation Remedial (Manual Welding and Semi-Automatic Welding) (cont.)

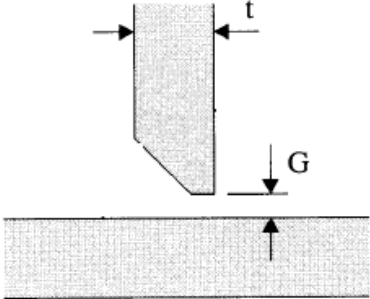
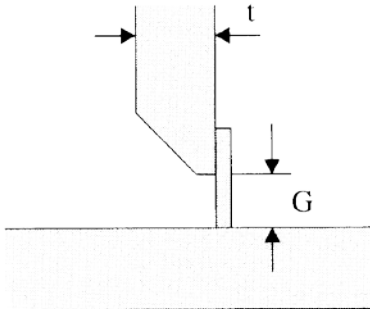
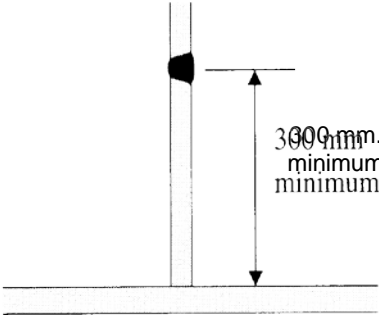
Detail	Remedial Standard	Remarks
<p>Single bevel tee</p> 	<p>$3\text{ mm} < G \leq 5\text{ mm}$ build up weld</p>	
	<p>$5\text{ mm} < G \leq 16\text{ mm}$ - build up with welding, with backing strip if necessary, remove backing strip if used, back gouge and back weld.</p> 	
	<p>$G > 16\text{ mm}$ new plate to be inserted of minimum width 300 mm</p> 	

Table 1.21 Typical Fillet Weld Plate Edge Preparation Remedial (Manual Welding and Semi-Automatic Welding) (cont.)

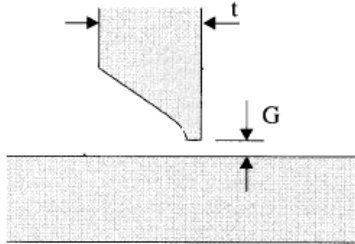
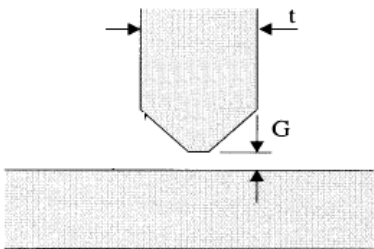

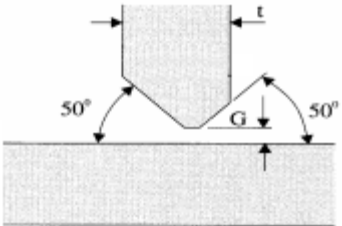
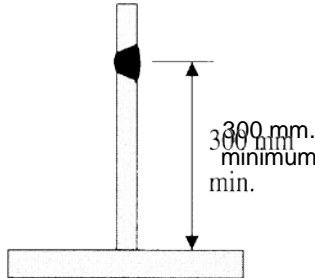
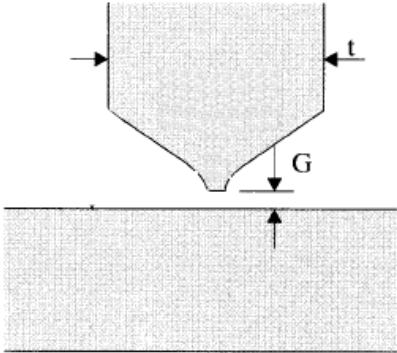
Detail	Remedial Standard	Remarks
<p>Single 'J' bevel tee</p> 	<p>as single bevel tee</p>	
<p>Double bevel tee symmetrical</p> 	<p>When $5 \text{ mm} < G \leq 16 \text{ mm}$ build up with welding using ceramic or other approved backing bar, remove, back gouge and back weld.</p> 	
<p>Double bevel tee asymmetrica</p> 	<p>When $G > 16 \text{ mm}$ insert plate of minimum height 300 mm to be fitted.</p> 	
<p>Double 'J' bevel symmetrical</p> 		

Table 1.22 Typical Fillet and Butt Weld Plate Edge Preparation Remedial (Manual Welding and Semi-Automatic Welding)

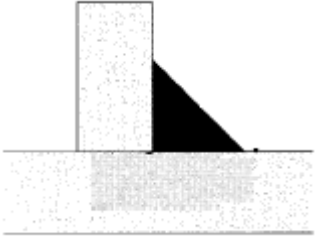
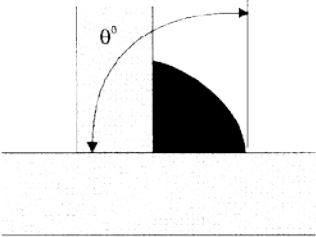
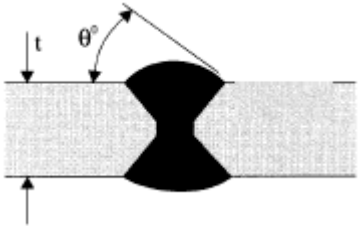
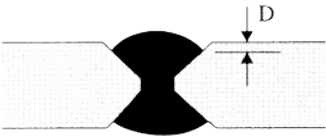

Detail	Remedial Standard	Remarks
<p>Fillet weld leg length</p> 	<p>Increase leg or throat by welding over</p>	
<p>Fillet weld toe angle</p> 	<p>$\theta > 90^\circ$ grinding, and welding, where necessary, to make $\theta \leq 90^\circ$</p>	<p>Minimum short bead to be referred Table 1.27</p>
<p>Butt weld toe angle</p> 	<p>$\theta > 90^\circ$ grinding, and welding, where necessary, to make $\theta \leq 90^\circ$</p>	
<p>Butt weld undercut</p> 	<p>For strength member, where $0.5 < D \leq 1$ mm, and for other, where $0.8 < D \leq 1$ mm, undercut to be ground smooth (localized only) or to be filled by welding</p> <p>Where $D > 1$ mm undercut to be filled by welding</p>	
<p>Fillet weld undercut</p> 	<p>Where $0.8 < D \leq 1$ mm undercut to be ground smooth (localized only) or to be filled by welding</p> <p>Where $D > 1$ mm undercut to be filled by welding</p>	

Table 1.23 Distance between welds remedial

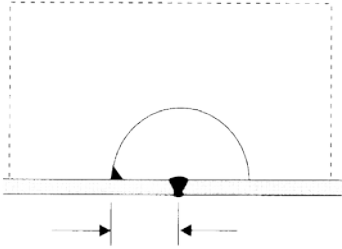
Detail	Remedial Standard	Remarks
<p data-bbox="167 304 448 331">Scallops over weld seams</p> 	<p data-bbox="651 439 1038 495">Hole to be cut and ground smooth to obtain distance</p>	

Table 1.24 Erroneous hole remedial

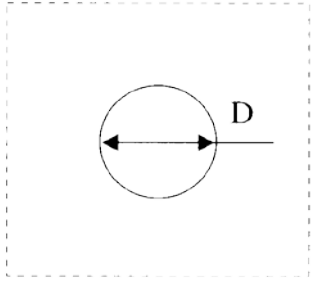
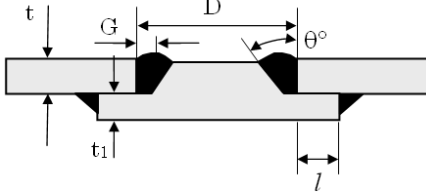
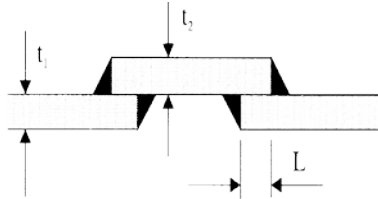
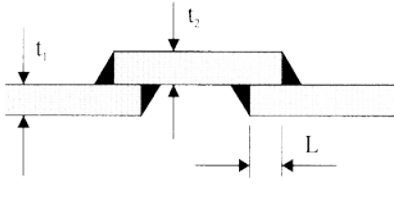
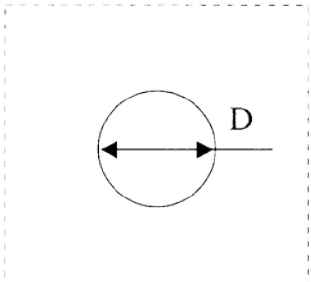
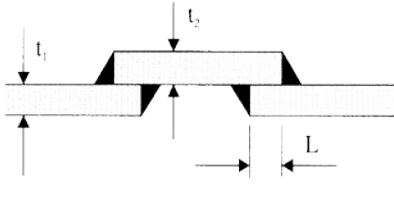
Detail	Remedial Standard	Remarks
<p>Holes made erroneously $D < 200$ mm</p> 	<p>Strength member open hole to minimum 75 mm dia., fit and weld spigot piece</p>  <p>$\theta = 30 - 40^\circ$ $G = 4 - 6$ mm $1/2t \leq t_1 \leq t$ $l = 50$ mm</p> <p>Or open hole to over 300 mm and fit insert plate</p>	<p>Fillet weld to be made after butt weld</p> <p>The fitting of spigot pieces in areas of high stress concentration or fatigue is to be approved by TL</p>
<p>Other open hole to over 300 mm and fit insert plate</p> <p>Or fit lap plate</p>  <p>$t_1 = t_2$ $L = 50$ mm, min</p>	<p>Strength member open hole and fit insert plate</p> <p>Other open hole to over 300 mm and fit insert plate</p> <p>Or fit lap plate</p>  <p>$t_1 = t_2$ $L = 50$ mm, min</p>	
<p>Holes made erroneously $D \geq 200$ mm</p> 	<p>Strength member open hole and fit insert plate</p> <p>Other open hole to over 300 mm and fit insert plate</p> <p>Or fit lap plate</p>  <p>$t_1 = t_2$ $L = 50$ mm, min</p>	

Table 1.25 Remedial by insert plate

Detail	Remedial Standard	Remarks
<p>Remedial by insert plate</p>	<p> $L = 300 \text{ mm minimum}$ $B = 300 \text{ mm minimum}$ $R = 5t \text{ mm}$ 100mm minimum </p> <p>(1) seam with insert piece is to be welded first</p> <p>(2) original seam is to be released and welded over for a minimum of 100 mm.</p>	
<p>Remedial of built section by insert plate</p>	<p> $L_{min} \geq 300 \text{ mm}$ </p> <p>Welding sequence $(1) \rightarrow (2) \rightarrow (3) \rightarrow (4)$ </p> <p>Web butt weld scallop to be filled during final pass (4)</p>	

Table 1.26 Weld surface remedial

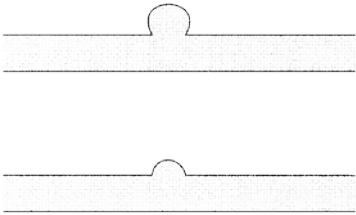
Detail	Remedial Standard	Remarks
<p>Weld spatter</p> 	<ol style="list-style-type: none"> 1. Remove spatter observed before blasting with scraper or chipping hammer, etc. 2. For spatter observed after blasting: <ol style="list-style-type: none"> a) Remove with a chipping hammer, scraper, etc. b) For spatter not easily removed with a chipping hammer, scraper, etc., grind the sharp angle of spatter to make it obtuse. 	<p>In principle, no grinding is applied to weld surface.</p>
<p>Arc strike</p> <p>(HT steel, Cast steel, Grade E of mild steel, TMCP type HT steel, Low temp steel)</p>	<p>Remove the hardened zone by grinding or other measures such as overlapped weld bead etc.</p>	<p>Minimum short bead to be referred Table 1.27</p>

Table 1.27 Welding remedial by short bead

Detail	Remedial Standard	Remarks
Short bead for remedying scar (scratch)	<p>a) HT steel, Cast steel, TMCP type HT steel (Ceq > 0.36%) and Low temp steel (Ceq > 0.36%)</p> <p>Length of short bead ≥ 50 mm</p> <p>b) Grade E of mild steel</p> <p>Length of short bead ≥ 30 mm</p> <p>c) TMCP type HT steel (Ceq ≤ 0.36%) and Low temp steel (Ceq ≤ 0.36%)</p> <p>Length of short bead ≥ 10 mm</p>	Preheating is necessary at 100 ± 25°C
Remedying weld bead	<p>a) HT steel, Cast steel, TMCP type HT steel (Ceq > 0.36%) and Low temp steel (Ceq > 0.36%)</p> <p>Length of short bead ≥ 50 mm</p> <p>b) Grade E of mild steel</p> <p>Length of short bead ≥ 30 mm</p> <p>c) TMCP type HT steel (Ceq ≤ 0.36%) and Low temp steel (Ceq ≤ 0.36%)</p> <p>Length of short bead ≥ 30 mm</p>	
<p>Note:</p> <p>1. When short bead is made erroneously, remove the bead by grinding.</p> <p>2. $Ceq = C + \frac{Mn}{6} + \frac{Cr + Mo + V}{5} + \frac{Ni + Cu}{15} (\%)$</p>		

REFERENCES

- A1. IACS Recommendation No.76 "Bulk Carriers - Guidelines for Surveys, Assessment and Repair of Hull Structure"
- A2. TSCF "Guidelines for the inspection and maintenance of double hull tanker structures"
- A3. TSCF "Guidance manual for the inspection and condition assessment of tanker structures"
- A4. IACS UR W7 "Hull and machinery steel forgings"
- A5. IACS UR W8 "Hull and machinery steel castings"
- A6. IACS UR W11 "Normal and higher strength hull structural steels"
- A7. IACS UR W13 "Thickness tolerances of steel plates and wide flats"
- A8. IACS UR W14 "Steel plates and wide flats with specified minimum through thickness properties ("Z" quality)"
- A9. IACS UR W17 "Approval of consumables for welding normal and higher strength hull structural steels"
- A10. IACS UR W28 "Welding procedure qualification tests of steels for hull construction and marine structures"
- A11. Annex I to IACS UR Z10.1 "Hull surveys of oil tankers", and Z10.2 "Hull surveys of bulk carriers", Z10.3 "Hull Surveys of Chemical Tankers", Z10.4 "Hull Surveys of Double Hull Oil Tankers" and Z10.5 "Hull Surveys of Double-Skin Bulk Carriers" Annex I
- A12. IACS UR Z23 "Hull survey for new construction"
- A13. IACS Recommendation No. 12 "Guidelines for surface finish of hot rolled plates and wide flats"
- A14. IACS Recommendation No. 20 "Non-destructive testing of ship hull steel welds"
- A15. IACS Recommendation No.96 "Double Hull Oil Tankers- Guidelines for Surveys, Assessment and Repair of Hull Structures"
- A16. IACS Recommendation No.55 "General Dry Cargo Ships- Guidelines for Surveys, Assessment and Repair of Hull Structures"
- A17. IACS Recommendation No.84 "Container Ships- Guidelines for Surveys, Assessment and Repair of Hull Structures"

SECTION 2**REPAIR QUALITY STANDARD FOR EXISTING SHIPS****Page**

A. SCOPE	2- 2
B. GENERAL REQUIREMENTS TO REPAIRS AND REPAIRERS	2- 2
C. QUALIFICATION OF PERSONNEL	2- 2
1. Qualification of welders	
2. Qualification of welding procedures	
3. Qualification of NDE operators	
D. MATERIALS	2- 3
1. General requirements to materials	
2. Equivalency of material grades	
E. GENERAL REQUIREMENTS TO WELDING	2- 4
1. Correlation of welding consumables to hull structural steels	
2. General requirements to preheating and drying out	
3. Dry welding on hull plating below the waterline of vessels afloat	
F. REPAIR QUALITY STANDARD	2- 8
1. Welding, general	
2. Renewal of plates	
3. Doubler on plates	
4. Renewal of internals/stiffeners	
5. Renewal of internals/stiffeners - transitions inverted angles/bulb profiles	
6. Application of Doubling Straps	
7. Welding of pitting corrosion	
8. Welding repairs of cracks	

A. Scope

1. This standard provides guidance on quality of repair of hull structures. The standard covers permanent repairs of existing ships.

Whereas the standard generally applies to

- Conventional ship types,
- Parts of hull covered by the rules of **TL**,
- Hull structures constructed from normal and higher strength hull structural steel,

The applicability of the standard is in each case to be agreed upon by **TL**.

The standard does generally not apply to repair of

- Special types of ships as e.g. gas tankers,
- Structures fabricated from stainless steel or other, special types or grades of steel.

2. The standard covers typical repair methods and gives guidance on quality standard on the most important aspects of such repairs. Unless explicitly stated elsewhere in the standard, the level of workmanship reflected herein will in principle be acceptable for primary and secondary structure of conventional design. A more stringent standard may however be required for critical and highly stressed areas of the hull and is to be agreed with **TL** in each case. **In assessing the criticality of hull structure and structural components, reference is made to ref. B1, B2, B3, B6, B10, B11 and B12.**

3. Restoration of structure to the original standard may not constitute durable repairs of damages originating from insufficient strength or inadequate detail design. In such cases strengthening or improvements beyond the original design may be required. Such improvements are not covered by this standard, however it is referred to **ref. B1, B2, B3, B6, B10, B11 and B12.**

B. General Requirements for Repairs and Repairers

1. In general, when hull structure covered by classification is to be subjected to repairs, the work is to be carried out under the supervision of the Surveyor to **TL**. Such repairs are to be agreed prior to commencement of the work.

2. Repairs are to be carried out by workshops, repair yards or personnel who have demonstrated their capability to carry out hull repairs of adequate quality in accordance with **TL** requirements and this standard.

3. Repairs are to be carried out under working conditions that facilitate sound repairs. Provisions are to be made for proper accessibility, staging, lighting and ventilation. Welding operations are to be carried out under shelter from rain, snow and wind.

4. Welding of hull structures is to be carried out by qualified welders, according to approved and qualified welding procedures and with welding consumables approved by **TL**, see C. Welding operations are to be carried out under proper supervision of the repair yard.

5. Where repairs to hull which affect or may affect classification are intended to be carried out during a voyage, complete repair procedure including the extent and sequence of repair is to be submitted to and agreed upon by the Surveyor to **TL** reasonably in advance of the repairs. **See ref. B7.**

C. Qualification of Personnel

1. Qualification of Welders

1.1 Welders are to be qualified in accordance with the procedures of **TL** or to a recognised national or international standard, e.g. EN 287, ISO 9606, ASME Section IX, ANSI/AWS D1.1. Recognition of other standards is subject to submission to **TL** for evaluation. Repair yards and workshops are to keep records of welders qualification and, when required, furnish valid approval test certificates.

1.2 Welding operators using fully mechanised or fully automatic processes need generally not pass approval testing, provided that production welds made by the operators are of the required quality. However, operators are to receive adequate training in setting or programming and operating the equipment. Records of training and production test results shall be maintained on individual operator's files and records, and be made available to **TL** for inspection when requested.

2. Qualification of Welding Procedures

Welding procedures are to be qualified in accordance with the procedures of **TL** or a recognised national or international standard, e.g. EN288, ISO 9956, ASME Section IX, ANSI/AWS D1.1. Recognition of other standards is subject to submission to **TL** for evaluation. The welding procedure should be supported by a welding procedure qualification record. The specification is to include the welding process, types of electrodes, weld shape, edge preparation, welding techniques and positions

3. Qualification of NDE Operators

3.1 Personnel performing non destructive examination for the purpose of assessing quality of welds in connection with repairs covered by this standard, are to be qualified in accordance with **TL** rules or to a recognised international or national qualification scheme. Records of operators and their current certificates are to be kept and made available to the Surveyor for inspection.

D. Materials

1. General Requirements for Materials

1.1 The requirements for materials used in repairs are in general the same as the requirements for materials specified in **TL** rules for new constructions (ref. B4).

1.2 Replacement material is in general to be of the same grade as the original approved material. Alternatively, material grades complying with recognised national or international standards maybe accepted by

TL provided such standards give equivalence to the requirements of the original grade or are agreed by **TL**.

For assessment of equivalency between steel grades, the general requirements and guidelines in item 2 apply.

1.3 Higher tensile steel is not to be replaced by steel of a lesser strength unless specially approved by **TL**.

1.4 Normal and higher strength hull structural steels are to be manufactured at works approved by **TL** for the type and grade being supplied.

1.5 Materials used in repairs are to be certified by **TL** applying the procedures and requirements in the rules for new constructions. In special cases, and normally limited to small quantities, materials may be accepted on the basis of alternative procedures for verification of the material's properties. Such procedures are subject to agreement by **TL** in each separate case.

2. Equivalency of Material Grades

2.1 Assessment of equivalency between material grades should at least include the following aspects;

- Heat treatment/delivery condition,
- Chemical composition,
- Mechanical properties,
- Tolerances.

2.2 When assessing the equivalence between grades of normal or higher strength hull structural steels up to and including grade E40 in thickness limited to 50 mm, the general requirements in Table 2.1 apply.

2.3 Guidance on selection of steel grades to certain recognised standards equivalent to hull structural steel grades specified in **TL** rules is given in Table 2.2

E. General Requirements to Welding**1. Correlation of Welding Consumables with Hull Structural Steels**

1.1 For the different hull structural steel grades welding consumables are to be selected in accordance with IACS UR W17 (see ref.B5).

1.2 General requirements to preheating and drying out

1.2.1 The need for preheating is to be determined based on the chemical composition of the materials, welding process and procedure and degree of joint restraint.

1.2.2 A minimum preheat of 50°C is to be applied when ambient temperature is below 0°C. Dryness of the welding zone is in all cases to be ensured.

1.2.3 Guidance on recommended minimum preheating temperature for higher strength steel is given in Table 2.3. For automatic welding processes utilising higher heat input e.g. submerged arc welding, the temperatures may be reduced by 50°C. For re-welding or

repair of welds, the stipulated values are to be increased by 25°C.

1.3 Dry welding on hull plating below the waterline of vessels afloat

1.3.1 Welding on hull plating below the waterline of vessels afloat is acceptable only on normal and higher strength steels with specified yield strength not exceeding 355 MPa and only for local repairs. Welding involving other high strength steels or more extensive repairs against water backing is subject to special consideration and approval by TL of the welding procedure.

1.3.2 Low-hydrogen electrodes or welding processes are to be used when welding on hull plating against water backing. Coated low-hydrogen electrodes used for manual metal arc welding should be properly conditioned to ensure a minimum of moisture content.

1.3.3 In order to ensure dryness and to reduce the cooling rate, the structure is to be preheated by a torch or similar prior to welding, to a temperature of minimum 5°C or as specified in the welding procedure.

Table 2.1 Minimum extent and requirements to assessment of equivalency between normal or higher strength hull structural steel grades

Items to be considered	Requirements	Comments
Chemical composition	<ul style="list-style-type: none"> - C; equal or lower - P and S; equal or lower - Mn; approximately the same but not exceeding 1.6% - Fine grain elements; in same amount - Deoxidation practice 	The sum of the elements, e.g. Cu, Ni, Cr and Mo should not exceed 0.8%
Mechanical properties	<ul style="list-style-type: none"> - Tensile strength; equal or higher - Yield strength; equal or higher - Elongation; equal or higher - Impact energy; equal or higher at same or lower temperature, where applicable 	Actual yield strength should not exceed TL Rule minimum requirements by more than 80 N/mm ²
Condition of supply	Same or better	Heat treatment in increasing order; <ul style="list-style-type: none"> - as rolled (AR) - controlled rolled (CR) - normalised (N) - thermo-mechanically rolled (TM) (1) - quenched and tempered (QT) (1)
Tolerances	Same or stricter	Permissible under thickness tolerances; <ul style="list-style-type: none"> - plates: 0.3 mm - sections: according to recognised standards
<p><i>Note :</i> (1) <i>TM- and QT-steels are not suitable for hot forming</i></p>		

Table 2.2 Guidance on steel grades comparable to the normal and high strength hull structural steel grades given in TL rules

Steel grades according to TL rules (ref. B4)						Comparable steel grades (1)			
Grade	Yield stress ReH min. N/mm ²	Tensile strength Rm N/mm ²	Elongation A5 min. %	Average impact energy for t ≤ 50 mm		EN 10025:1990 (2) ISO 4950-2:1995	EN 10025 Series:2004	ASTMA 131 GB712-2011	JIS G 3106
				Test temp. °C	J, min. L T				
A B D E	235	400 - 520	22	+20 0 -20 -40	- - 27 20 27 20 27 20	Fe 360B Fe 360C Fe 360D -	S235JR S235J0 S235J2 S275NL, S275ML	A B D E	SM400B SM400B, SM400C -
A 27 D 27 E 27	265	400 - 530	22	0 -20 -40	27 20	Fe 430C Fe 430D -	S275J0 S275J2, S275N/S275M S275NL, S275ML	- - -	- - -
A 32 D 32 E 32	315	440 - 570	22	0 -20 -40	31 22	- - -	- - -	AH32 DH32 EH32	SM490B, SM490C - -
A 36 D 36 E 36	355	490 - 630	21	0 -20 -40	34 24	Fe 510C Fe510D E355DD	S355J0 S355J2, S355N, S355 M S355NL, S355ML	AH36 DH36 EH36	SM520B, SM520C - -
A 40 D 40 E 40	390	510 - 660	20	0 -20 -40	39 26	E390CC E390DD E390E	S420N S420M S420N/S420M S420NL, S420ML	AH40 DH40 EH40	SM570 - -

Note :

(1) In selecting comparable steels from this table, attention should be given to the requirements of Table 2.1 and the dimension requirements of the product with respect to TL rules. Some steel grades as per national or international standard are defined with specified yield and tensile strength properties which depend on thickness. For thicknesses with tensile properties specified lower than those of TL Rules, case-by-case consideration shall be given with regards to design requirements.

(2) EN 10025:1990 is superseded by EN10025 series.


Table 2.3 Preheating temperature

Carbon equivalent (1)	Recommended minimum preheat temperature (°C)		
	$t_{comb} \leq 50$ mm (2)	50 mm $< t_{comb} \leq 70$ mm (2)	$t_{comb} > 70$ mm (2)
$C_{eq} \leq 0.39$	-	-	-
$C_{eq} \leq 0.41$	-	-	-
$C_{eq} \leq 0.43$	-	50	100
$C_{eq} \leq 0.45$	50	100	125
$C_{eq} \leq 0.47$	100	125	150
$C_{eq} \leq 0.50$	125	150	175

Notes :

(1)
$$C_{eq} = C + \frac{Mn}{6} + \frac{Cr + Mo + V}{5} + \frac{Ni + Cu}{15} (\%)$$

(2) Combined thickness $t_{comb} = t_1 + t_2 + t_3 + t_4$, see figure

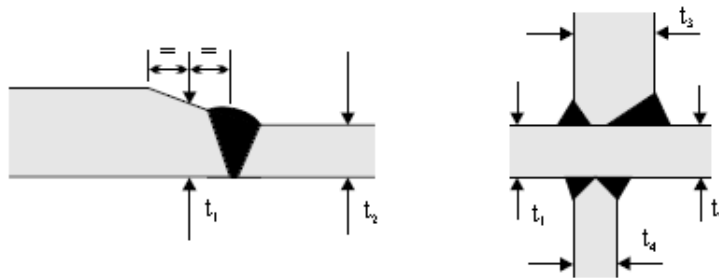

F. Repair Quality Standard

1. Welding, General

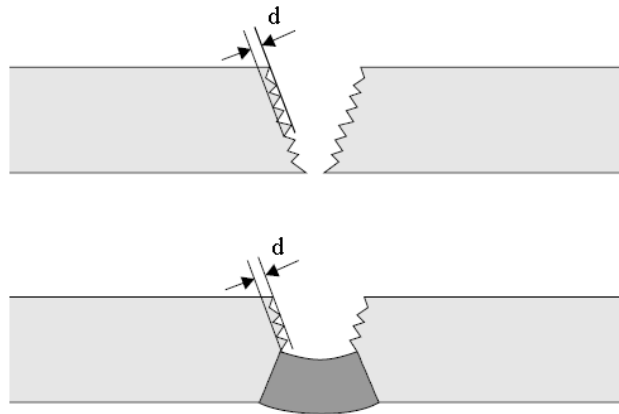


Figure 2.1 Groove roughness

Table 2.4 Repair quality

Item	Standard	Limit	Remarks
Material Grade	Same as original or higher		See D.
Welding Consumables	IACS UR-W17 (ref. B5)	Approval according to equivalent international standard	
Groove / roughness	See note and Fig. 2.1	$d < 1.5 \text{ mm}$	Grind smooth
Pre-Heating	See Table 2.3	Steel temperature not lower than 5°C	
Welding with water on the outside	See E.1.3	Acceptable for normal and high strength steels	Moisture to be removed by a heating torch
Alignment	As for new construction		
Weld finish	IACS Rec. 20 (ref. B9)		
NDE	IACS Rec. 20 (ref. B9)	At random with extent to be agreed with attending surveyors	
<p><i>Note :</i> Slag, grease, loose mill scale, rust and paint, other than primer, to be removed</p>			

2. Renewal of plates

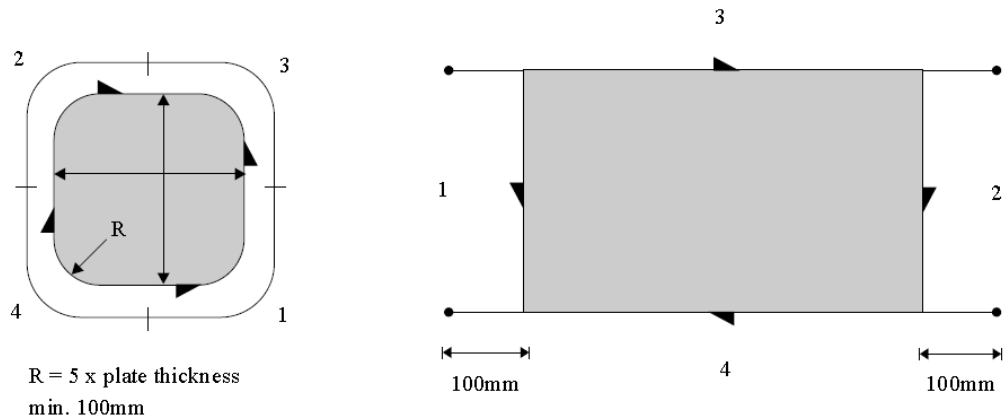


Figure 2.2 Welding sequence for inserts

Table 2.5 Renewal of plates

Item	Standard	Limit	Remarks
Size insert	Min. 300x300mm R = 5 x thickness Circular inserts: D _{min} =200mm	Min. 200x200mm Min R = 100 mm	
Material grade	Same as original or higher		See D.
Edge Preparation	As for new construction		In case of non compliance increase the amount of NDE
Welding sequence	See Fig.2.2 Weld sequence is 1→ 2→ 3→ 4		For primary members sequence 1 and 2 transverse to the main stress direction
Alignment	As for new construction		
Weld finish	IACS Rec. 20 (ref. B9)		
NDE	IACS Rec. 20 (ref. B9)		

3. Doublers on plating

Local doublers are normally only allowed as temporary repairs, except as original compensation for openings, within the main hull structure

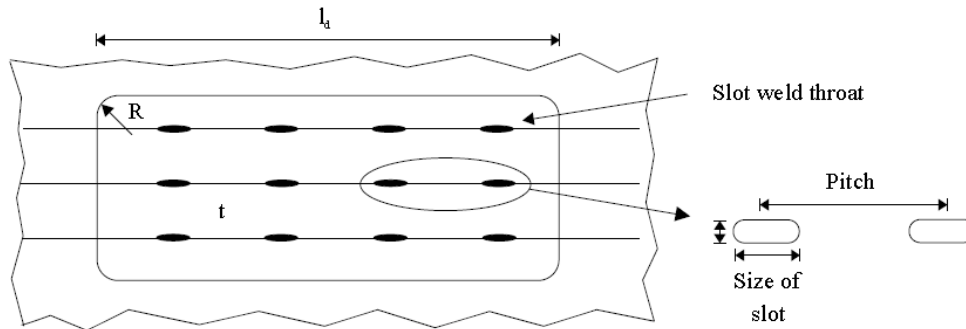


Fig. 2.3 Doublers on plates

Table 2.6 Doublers on plates

Item	Standard	Limit	Remarks
Existing plating		General: $t \geq 5 \text{ mm}$	For areas where existing plating is less than 5mm plating a permanent repair by insert is to be carried out.
Extent/size	Rounded off corners.	min 300x300 mm $R \geq 50\text{mm}$	
Thickness of doubler (t_d)	$t_d \leq t_p$ (t_p =original thickness of existing plating)	$t_d > t_p/3$	
Material grade	Same as original plate		See D.
Edge preparation	As for [new building] new construction		Doublers welded on primary strength members: (L_e : leg length) when $t > L_e + 5\text{mm}$, the edge to be tapered (1:4)
Welding	As for [new building] new construction		Welding sequence similar to insert plates.
Weld size(throat thickness)	Circumferential and in slots: $0.6 \times t_d$		
Slot welding	Normal size of slot: (80-100) x $2 t_d$ Distance from doubler edge and between slots: $d \leq 15 t_d$	Max pitch between slots 200mm $d_{\text{max}} = 500\text{mm}$	For doubler extended over several supporting elements, see Figure 2.3
NDE	IACS Rec. 20 (ref. B9)		

4. Renewal of internals / stiffeners

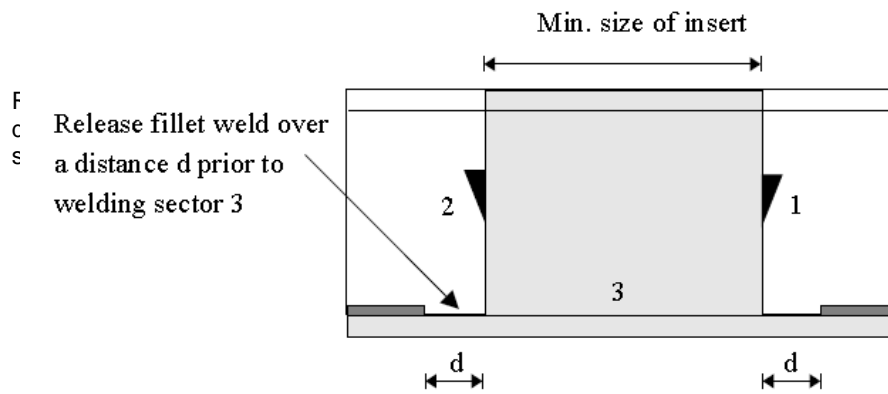


Figure 2.4 Welding sequence for inserts of stiffeners

Table 2.7 Renewals of internals / stiffeners

Item	Standard	Limit	Remarks
Size insert	Min. 300 mm	Min. 200mm	
Material grade	Same as original or higher		See D.
Edge Preparation	As for new construction. Fillet weld stiffener web/plate to be released over min. $d = 150$ mm		
Welding sequence	See Fig.2.4 Weld sequence is $1 \rightarrow 2 \rightarrow 3$		
Alignment	As for new construction		
Weld finish	IACS Rec. 20 (ref. B9)		
NDE	IACS Rec. 20 (ref. B9)		

5. Renewal of internals/stiffeners - transitions inverted angle/bulb profile

The application of the transition is allowed for secondary structural elements

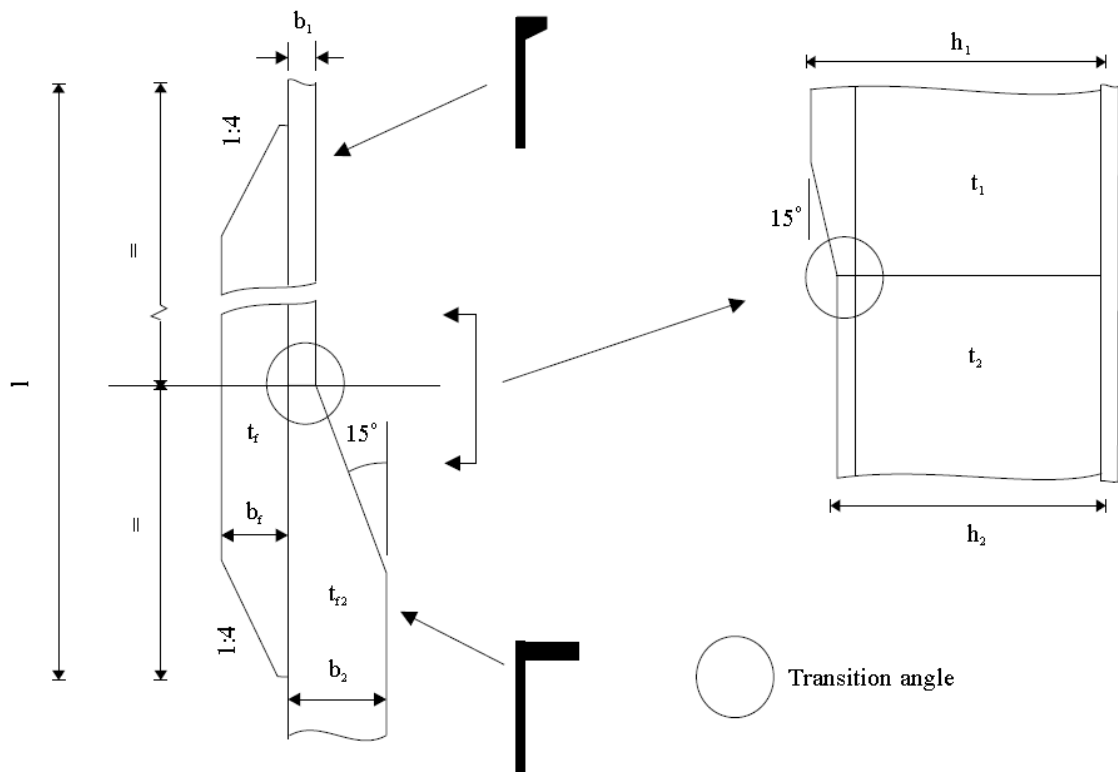


Figure 2.5 Transition between inverted angle and bulb profile

Table 2.8 Renewal of internals/stiffeners - transitions inverted angle/bulb profile

Item	Standard	Limit	Remarks
$(h_1 - h_2)$	$\leq 0.25 \times b_1$		
$ t_1 - t_2 $	2 mm		Without tapering transition.
Transition angle	15 degrees		At any arbitrary section
Flanges	$t_f = t_{f2}$ $b_f = b_{f2}$		
Length of flatbar	$4 \times h_1$		
Material			See D.

6. Application of Doubling Straps

In certain instances, doubling straps are used as a means to strengthen and reinforce primary structure. Where this has been agreed and approved, particular attention should be paid to:

- The end termination points of the straps, so that toe support is such that no isolated hard point occurs.
- In the case of application of symmetrical or asymmetrical-ended straps, the corners at the end of the tapering should be properly rounded.
- Any butts between lengths of doubling straps, so that there is adequate separation of the butt weld from the primary structure below during welding, and so that a high quality root run under controlled circumstances is completed prior to completing the remainder of the weld. Ultrasonic testing should be carried out on completion to verify full penetration.

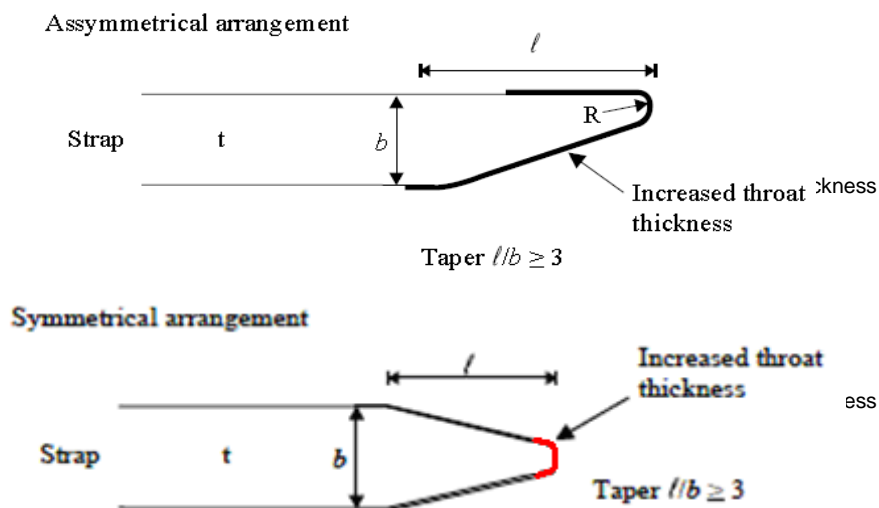


Figure 2.6 Application of doubling straps

Table 2.6 Termination of straps

Item	Standard	Limit	Remarks
Tapering	$l/b > 3$		Special consideration to be drawn to design of strap terminations in fatigue sensitive areas.
Radius	$0.1 \times b$	min 30 mm.	
Material			See D. General requirement to materials.
Weld size			Depending on number and function of straps. Throat thickness to be increased 15 % toward ends.
Welding	Welding sequence from middle towards the free ends		See sketch. For welding of lengths > 1000 mm step welding to be applied.

7. Welding of pitting corrosion

Notes:

Shallow pits may be filled by applying coating or pit filler. Pits can be defined as shallow when their depth is less than 1/3 of the original plate thickness

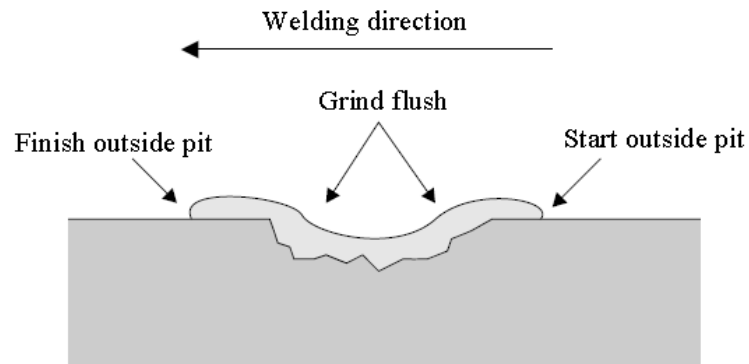


Figure 2.7 Welding of pits

Table 2.10 Welding of pitting corrosion

Item	Standard	Limit	Remarks
Extent/depth	Pits/grooves are to be welded flush with the original surface.	If deep pits or grooves are clustered together or remaining thickness is less than 6 mm, the plate should be renewed.	IACS Rec. 12 (ref.B8)
Cleaning	Heavy rust to be removed		
Pre-Heating	See Table 2.3	Required when ambient temperature < 5°C	Always use propane torch or similar to remove any moisture
Welding sequence	Reverse direction for each layer		IACS Rec. 12 (ref.B8)
Weld finish	IACS Rec. 20 (ref.B9)		
NDE	IACS Rec. 20 (ref.B9)	Min. 10% extent	Preferably MPI
Reference is made to TSCF Guideline, Ref.B2 & B3			

8. Welding repairs for cracks

In the event that a crack is considered weldable, either as a temporary or permanent repair, the following techniques should be adopted as far as practicable. Run-on and run-off plates should be adopted at all free edges.

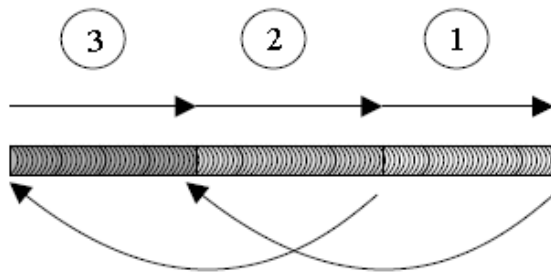


Fig. 6.8.a Step back technique

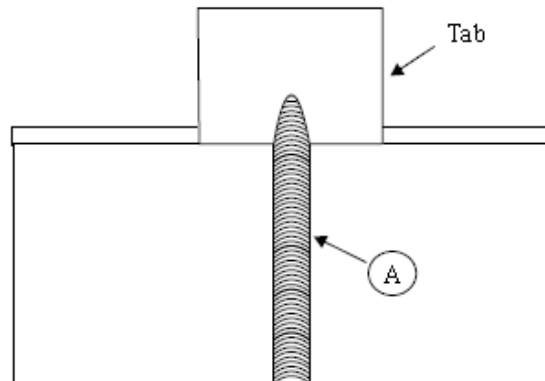


Fig 6.8.b End crack termination

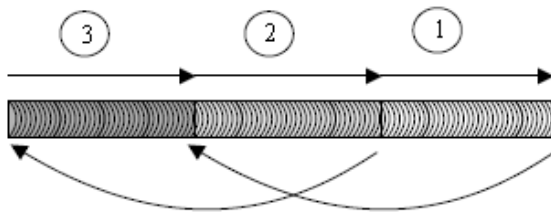


Fig 6.8.c Welding sequence for cracks with length less than 300 mm

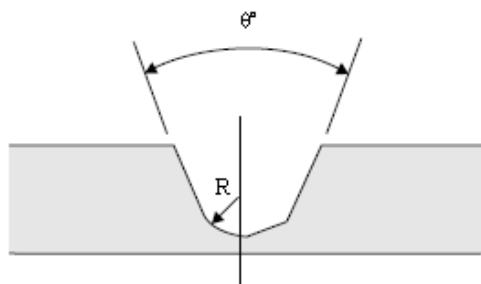
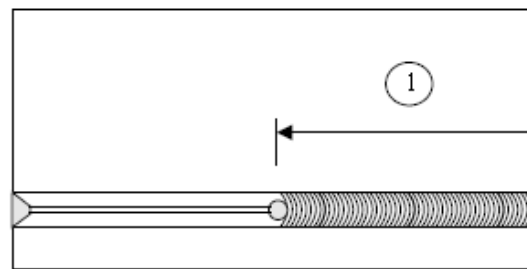


Fig. 6.8.d Groove preparation
(U-groove left and V-groove right)

Table 2.11 Welding repairs for cracks

Item	Standard	Limit	Remarks
Groove preparation	$\theta=45-60^\circ$ $r=5\text{ mm}$		For through plate cracks as for newbuilding. Also see Fig. 2.11
Termination	Termination to have slope 1:3		For cracks ending on edges weld to be terminated on a tab see Fig.2.9
Extent	On plate max. 400 mm length. Vee out 50 mm past end of crack	On plate max 500 mm. Linear crack, not branched	
Welding sequence	See Fig. 2.10 for sequence and direction	For cracks longer than 300 mm step- back technique should be used Fig.2.8	Always use low hydrogen welding consumables
Weld finish	IACS Rec. 20 (ref.B9)		
NDE	IACS Rec. 20 (ref.B9)	100 % MP or PE of groove	100 % surface crack detection + UE or RE for butt joints

REFERENCES

- B1. IACS Recommendation 76 “Bulk Carriers - Guidelines for Surveys, Assessment and Repair of Hull Structure”
- B2. TSCF “Guidelines for the inspection and maintenance of double hull tanker structures”
- B3. TSCF “Guidance manual for the inspection and condition assessment of tanker structures”
- B4. IACS UR W11 “Normal and higher strength hull structural steels”
- B5. IACS UR W17 “Approval of consumables for welding normal and higher strength hull structural steels”
- B6. Annex I to IACS Z10.1 “Hull surveys of oil tankers”, and Z10.2 “Hull surveys of bulk carriers”, Z10.3 “Hull Surveys of Chemical Tankers”, Z10.4 “Hull Surveys of Double Hull Oil Tankers” and “Z10.5 Hull Surveys of Double-Skin Bulk Carriers” Table IV
- B7. IACS UR Z3 “Voyage repairs and maintenance”
- B8. IACS Recommendation 12 “Guidelines for surface finish of hot rolled steel plates and wide flats”
- B9. IACS Recommendation 20 “Non-destructive testing of ship hull steel welds”
- B10. IACS Recommendation No.96 “Double Hull Oil Tankers- Guidelines for Surveys, Assessment and Repair of Hull Structures”
- B11. IACS Recommendation No.55 “General Dry Cargo Ships- Guidelines for Surveys, Assessment and Repair of Hull Structures”
- B12. IACS Recommendation No.84 “Container Ships- Guidelines for Surveys, Assessment and Repair of Hull Structures”